English

Operating Manual

Calibration Baths

FK30-SL

FK31-SL

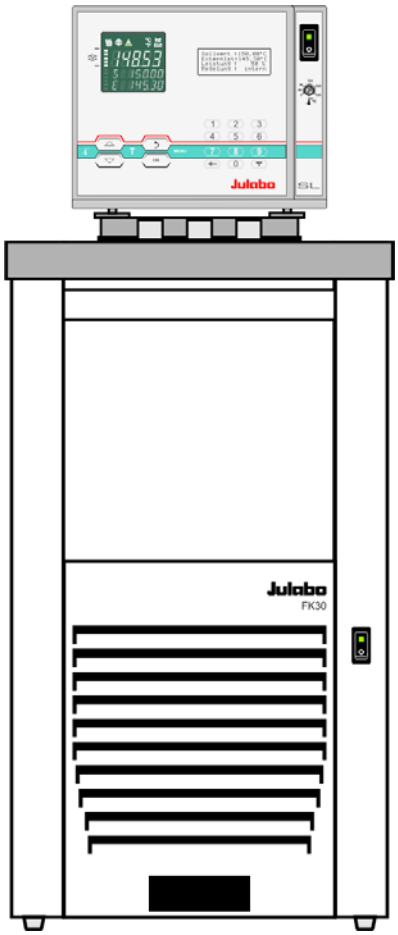

Julabo
THE TEMPERATURE CONTROL COMPANY

JULABO GmbH
77960 Seelbach / Germany
Tel. +49 (0) 7823 / 51-0
Fax +49 (0) 7823 / 24 91
info@julabo.de
www.julabo.de

1.951.2829-V2 **06/13**

19512829-V2.doc 22.07.13

Congratulations!

You have made an excellent choice.
JULABO thanks you for the trust you have placed in us.
This operating manual has been designed to help you gain an understanding of the operation and possible applications of our circulators. For optimal utilization of all functions, we recommend that you thoroughly study this manual prior to beginning operation.

The JULABO Quality Management System

Temperature control devices for research and industry are developed, produced, and distributed according to the requirements of ISO 9001 and ISO 14001. Certificate Registration No. 01 100044846

Unpacking and inspecting

Unpack the circulator and accessories and inspect them for possible transport damage. Damage should be reported to the responsible carrier, railway, or postal authority, and a damage report should be requested. These instructions must be followed fully for us to guarantee our full support of your claim for protecting against loss from concealed damage. The form required for filing such a claim will be provided by the carrier.

Printed in Germany Changes without prior notification reserved

Important: keep operation manual for future use

TABLE OF CONTENTS

Operating manual 5
1. Intended use 5
1.1. Description 5
2. Operator responsibility – Safety recommendations 6
2.1. Disposal 8
2.2. EC Conformity 9
2.3. Warranty conditions 9
2.4. Technical specifications 10
Operating instructions 12
3. Safety notes for the user 12
3.1. Explanation of safety notes 12
3.2. Explanation of other notes 12
3.3. Safety recommendations 13
4. Operating controls and functional elements 15
5. Preparations 19
5.1. Installation 19
5.2. Bath fluids 20
5.3. Filling / draining 21
6. Operating procedures 22
6.1. Power connection 22
6.2. Switching on / Selecting the language 22
6.2.1. Switching on the cooling machine 23
6.3. Start - Stop 23
6.4. Adjusting the temperature chamber 23
7. T Setting of temperatures 24
8. Safety installations, warning functions 24
8.0.1. Early warning system, low level protection 28
9. MENU Menu functions 29
9.1. Start of a program 31
9.1.1. Status at the end of a program 33
9.1.2. Indication after successful start 33
9.1.3. Editing after Start 34
9.1.4. Interrupting a program 34
9.1.5. Interruption after a power failure 35
9.1.6. Termination of a program 35
9.2. Program administration, creation 36
9.3. Setting the pump pressure 40
9.4. Configuration 41
9.4.1. Remote control via the serial interface 44
9.4.2. Keypad control or setpoint setting via the analog input 44
9.4.3. Autostart 45
9.4.4. Off-Mode 45

9.4.5. ActVar - actuating variable 46
9.4.6. Setting of clock and date 47
9.4.7. Language 47
9.4.8. Unit 47
9.4.9. Program type 47
9.4.10. Reset 47
9.4.11. C-Sensor - Precision reference sensor 48
9.5. Control 49
9.5.1. Control internal / external 51
9.5.2. Selftuning 52
9.5.3. Dynamik intern 52
9.5.4. CoSpeed - extern 53
9.5.5. Control parameters – internal/external 53
9.6. Serial Interface 55
9.7. ATC Absolute Temperature Calibration, 3-point calibration 56
9.7.1. ATC Fühler - intern / extern 59
9.7.2. ATC Status - yes / no 59
9.7.3. Type 1 -/ 2 -/ 3 point 59
9.7.4. Example: 3-point calibration for internal control 60
9.8. Limits 62
9.8.1. Limits for internal control and external control 63
9.8.2. Limits for external control 64
9.9. Analog inputs/outputs 65
9.9.1. Outputs of the connector - REG+E-PROG 69
9.9.2. Input of the connector - REG+E-PROG 70
9.9.3. External Stand-by input 72
9.9.4. Alarm-output 73
10. Troubleshooting guide / Error messages 74
11. Electrical connections 77
12. Remote control 80
12.1. Setup for remote control 80
12.2. Communication with a PC or a superordinated data system 80
12.3. List of commands 81
12.4. Status messages 85
12.5. Error messages 85
13. Installation of electronic module with analog connectors 86
14. JULABO Service – Online remote diagnosis 87
15. Cleaning / repairing the unit 88

Operating manual

1. Intended use

JULABO circulators have been designed to control the temperature of specific fluids in a bath tank.

	JULABO circulators are not suitable for direct temperature control of foods, semi-luxury foods and tobacco, or pharmaceutical and medical products. Direct temperature control means unprotected contact of the object with the bath medium (bath fluid).

1.1. Description



☑ The circulators are operated via the splash-proof keypad. The implemented microprocessor technology allows to set and to store different values that can be indicated on the VFD COMFORT-DISPLAY and LCD DIALOG-DISPLAY. Three menu keys facilitate adjusting setpoints, warning and safety functions and menu functions.



☑ The integrated programmer allows storing and running temperature and time-dependent processes.



☑ The control electronics including “ICC - Intelligent Cascade Control“ automatically adapts the heat supplied to the thermal requirements of the bath.

☑ The TCF - **T**emperature **C**ontrol **F**eatures allow the user to have access to all important temperature control parameters. This means: Full control on the control mode and the chance to manually adjust or adapt control to the specific application.

☑ Absolute Temperature Calibration (ATC3) provides high temperature stability in the bath. With the 3-point calibration an offset is adjusted at three temperatures to ensure an accurate temperature pattern at the selected spot in the bath over the full temperature range.



☑ Electrical connections:
The serial interface, switchable from RS232 to RS485, allows modern process technology without additional interface.
Connection for Pt100 external sensor for external temperature measurement and control.
Alarm output for external alarm message or control of JULABO refrigerating baths or solenoid valve (cooling water).
The electronic module (option) provides 3 further analog connections (alarm input, standby input, recorder output, programmer input).



☑ The excess temperature protection conforming to IEC 61010-2-010 is a safety installation independent from the control circuit. This protection can be indicated and set on the LCD DIALOG-DISPLAY.



☑ The early warning system for low level signals that bath fluid needs to be refilled before the low level protection conforming to IEC 61010-2-010 causes a complete shut-down of the main functional elements.

☑ Intelligent pump system: The pump capacity (electronically adjustable via the motor speed) enables to adapt to varying conditions for internal and external temperature applications.

2. Operator responsibility – Safety recommendations

The products of JULABO ensure safe operation when installed, operated, and maintained according to common safety regulations. This section explains the potential dangers that may arise when operating the circulator and also specifies the most important safety precautions to preclude these dangers as far as possible.

- The operator is responsible for the qualification of the personnel operating the units.
- The personnel operating the units should be regularly instructed about the dangers involved with their job activities as well as measures to avert these dangers.
- Make sure all persons tasked with operating, installing, and maintaining the unit have read and understand the safety information and operating instructions.
- When using hazardous materials or materials that could become hazardous, the circulator may be operated only by persons who are absolutely familiar with these materials and the circulator. These persons must be fully aware of possible risks.

If you have any questions concerning the operation of your unit or the information in this manual, please contact us!

Contact JULABO GmbH
Eisenbahnstraße 45
77960 Seelbach / Germany

Tel. +49 (0) 7823 / 51-0
Fax +49 (0) 7823 / 24 91
info@julabo.de
www.julabo.de

Safety instructions for the operator:

- You have received a product designed for industrial use. Nevertheless, avoid strikes to the housing, vibrations, damage to the operating-element panel (keypad, display), and contamination.
- Make sure the product is checked for proper condition regularly (depending on the conditions of use). Regularly check (at least every 2 years) the proper condition of the mandatory, warning, prohibition and safety labels.
- Make sure that the mains power supply has low impedance to avoid any negative effects on instruments being operated on the same mains.
- This unit is designed for operation in a controlled electromagnetic environment. This means that transmitting devices (e.g., cellular phones) should not be used in the immediate vicinity. Magnetic radiation may affect other devices with components sensitive to magnetic fields (e.g., monitors). We recommend maintaining a minimum distance of 1 m.
- Permissible ambient temperature: max. 40 °C, min. 5 °C.
- Permissible relative humidity: 50% (40 °C).
- Do not store the unit in an aggressive atmosphere.
- Protect the unit from contamination.
- Do not expose the unit to sunlight.

Appropriate operation

Only qualified personnel is authorized to perform configuration, installation, maintenance and repairs of the circulator.
Routine operation can also be carried out by untrained personnel who should however be instructed by trained personnel.

Use:

The bath can be filled with flammable materials. Fire hazard!
There might be chemical dangers depending on the bath medium used.
Observe all warnings for the used materials (bath fluids) and the respective instructions (safety data sheets).
Insufficient ventilation may result in the formation of explosive mixtures. Only use the unit in well ventilated areas.

Only use recommended materials (bath fluids). Only use non-acid and non corroding materials.

When using hazardous materials or materials that could become hazardous, **the operator must** affix the enclosed safety labels to the front of the unit so they are highly visible:

When using hazardous materials or materials that could become hazardous, **the operator must** affix the enclosed safety labels **(1 + 2)** to the front of the unit so they are highly visible:

1		Warning label W00: Colors: yellow, black Danger area. Attention! Observe instructions. (operating manual, safety data sheet)
2 **or**		Mandatory label M018: Colors: blue, white Carefully read the user information prior to beginning operation. **Scope: EU**
2		Semi S1-0701 Table A1-2 #9 Carefully read the user information prior to beginning operation. **Scope: USA, NAFTA**

Particular care and attention is necessary because of the wide operating range.
There are thermal dangers: Burn, scald, hot steam, hot parts and surfaces that can be touched.

		Warning label W26: Colors: yellow, black Hot surface warning. (The label is put on by JULABO)

Observe the instructions in the manuals for instruments of a different make that you connect to the circulator, particularly the respective safety recommendations. Also observe the pin assignment of plugs and technical specifications of the products.

2.1. Disposal

The circulator contains a back-up battery that supplies voltage to memory chips when the unit is switched off. Do not dispose of the battery with household waste!
Depending on battery regulations in your country, you might be obliged to give back used or defect batteries to gathering places.
The product may be used with oil as bath fluid. These oils fully or partially consist of mineral oil or synthetic oil. For disposal, observe the instructions in the safety data sheets.

This unit contains refrigerants, which at this time are not considered harmful to the ozone layer. However, over the long operating period of the unit, disposal rules may change. Therefore, only qualified personnel should handle the disposal.

Valid in EU countries
See the current official journal of the European Union – WEEE directive.
Directive of the European Parliament and of the Council on waste electrical and electronic equipment (WEEE).
This directive requires electrical and electronic equipment marked with a crossed-out trash can to be disposed of separately in an environmentally friendly manner.
Contact an authorized waste management company in your country.
Disposal with household waste (unsorted waste) or similar collections of municipal waste is not permitted!

2.2. EC Conformity

The products described in the operating instructions conform to the requirements of the following European guidelines:

Directive of the European Parliament and of the Council on the approximation of the laws of the Member States relating to machinery.

EMC guideline with respect to legal harmonization of the member countries concerning electromagnetic compatibility.

JULABO GmbH
Eisenbahnstr. 45
77960 Seelbach / Germany

2.3. Warranty conditions

JULABO GmbH warrants its products against defects in material or in workmanship, when used under appropriate conditions and in accordance with appropriate operating instructions

for a period of ONE YEAR.

Extension of the warranty period – free of charge

With the ‘1PLUS warranty’ the user receives a free of charge extension to the warranty of up to 24 months, limited to a maximum of 10 000 working hours.

To apply for this extended warranty the user must register the unit on the JULABO web site www.julabo.de, indicating the serial no. The extended warranty will apply from the date of JULABO GmbH’s original invoice.

JULABO GmbH reserves the right to decide the validity of any warranty claim. In case of faults arising either due to faulty materials or workmanship, parts will be repaired or replaced free of charge, or a new replacement unit will be supplied.

Any other compensation claims are excluded from this guarantee.

2.4. Technical specifications

Calibration Baths		**FK30-SL**	**FK31-SL**
Working temperature range	°C	-30 ... 200	-30 ... 200
Temperature stability [1]	°C	±0.005	±0.005
Temperature uniformity	°C	<±0.01	<±0.01
Cooling capacity	°C	+20 0 -20	+20 0 -20
Medium: ethanol	kW	0.46 0.34 0.15	0.46 0.34 0.15
Refrigerant		R134a	R134a
Overall dimensions (WxDxH)	cm	32x45x79	32x45x91
Bath opening (WxL)	cm	∅12	∅12
Bath depth	cm	17	31
Filling volume	Liter	14	24
Weight	kg	48	51
Mains power connection 230 V/50 Hz	V/ Hz	207-253 / 50	207-253 / 50
Current draw (at 230 V)	A	14	14
Current draw (at 230 V) <GB>	A	10 (Circulator)	10 (Circulator)
	A	4 (Cooling machine)	4 (Cooling machine)
Mains power connection 115 V/60 Hz	V/ Hz	103-127 / 60	103-127 / 60
Current draw (at 115 V)	A	10 (Circulator)	10 (Circulator)
	A	6 (Cooling machine)	6 (Cooling machine)

[1] ±0.02 °C@+200 °C

Circulator (SL-C)		**SL**
Temperature selection		digital
via keypad		indication on LCD DIALOG-DISPLAY (°C/°F)
remote control via PC		indication on monitor
Temperature indication		VFD COMFORT-DISPLAY (°C/°F)
Resolution	°C	0.01
ATC3 INT / EXT	°C	±3 / ±9
Temperature control		ICC - Intelligent Cascade Control
Heater wattage (at 230 V)	kW	2.0
Heater wattage (at 115 V)	kW	1.0
Electronically adj. pump capacity	stages	1 ... 4
Flow rate at 0 bar	l/min	22 ... 26
Max. pressure at 0 liters	bar	0.7
Max. suction at 0 liters	bar	0.4
Ambient temperature	°C	5 ... 40
Mains power connection 230 V/50-60 Hz	V/ Hz	190 ... 253 / 50-60
Current draw (at 208 V / 230 V)	A	12 / 13
Mains power connection 115 V/50-60 Hz	V/ Hz	90 ... 127 / 50-60
Current draw (at 100 V / 115 V)	A	9/10

All measurements have been carried out at: rated voltage and frequency
ambient temperature: 20 °C Technical changes without prior notification reserved.

Electrical connections:

External alarm device 24-0 V DC / max. 25 mA
Computer interface RS232 or RS485
External Pt100 sensor

Optional for HL, SL
(Order No. 8900100 Electronic module with analog connections)
Programmer input -100 °C to 400 °C = 0 - 10 V or 0 - 20 mA or 4 - 20 mA
Input for the signal of a flow meter or external manipulated variable
Temperature recorder outputs 0 - 10 V (0 V = -100 °C, 10 V = 400 °C)
0 - 20 mA (0 mA = -100 °C, 20 mA = 400 °C)
4 - 20 mA (4 mA = -100 °C, 20 mA = 400 °C)
Standby input for external emergency switch-off
Alarm output for external alarm signal

Safety installations according to IEC 61010-2-010:

Excess temperature protection	adjustable from 0 °C ... 320 °C
Low liquid level protection	float switch
Classification according to DIN 12876-1	class III

Supplementary safety installations

Early warning system for low level	float switch
High temperature warning function	optical + audible (in intervals)
Low temperature warning function	optical + audible (in intervals)
Supervision of working sensor	plausibility control
Reciprocal sensor monitoring between working and safety sensors	difference >35 K
Alarm message	optical + audible (permanent)
Warning message	optical + audible (in intervals)

Environmental conditions according to IEC 61 010-1:

Use indoors only.
Altitude up to 2000 m - normal zero.
Ambient temperature: see Technical specifications
Humidity:
Max. relative humidity 80% for temperatures up to +31 °C,
linear decrease down to 50% relative humidity at a temperature of +40 °C
Max. mains voltage fluctuations of ±10% are permissible.

Protection class according to IEC 60 529	IP21
The unit corresponds to Class I	
Overvoltage category	II
Pollution degree	2

Caution:
The unit is not suitable for use in explosive environment

EMC requirements according to EN 61326-1
This unit is an ISM device classified in Group 1 (using high frequency for internal purposes), Class A (industrial and commercial range).

Operating instructions

3. Safety notes for the user

3.1. Explanation of safety notes

	In addition to the safety warnings listed, warnings are posted throughout the operating manual. These warnings are designated by an exclamation mark inside an equilateral triangle. “Warning of a dangerous situation (Attention! Please follow the documentation).” The danger is classified using a signal word. Read and follow these important instructions for averting dangers.
	Warning: Describes a **possibly** highly dangerous situation. If these instructions are not followed, serious injury and danger to life could result.
	Caution: Describes a **possibly** dangerous situation. If this is not avoided, slight or minor injuries could result. A warning of possible property damage may also be contained in the text.
	Notice: Describes a **possibly** harmful situation. If this is not avoided, the product or anything in its surroundings can be damaged.

3.2. Explanation of other notes

	Note! Draws attention to something special.
	Important! Indicates usage tips and other useful information.
	This icon is used in the operating instructions to indicate flashing values or parameters which have to be set or confirmed.

3.3. Safety recommendations

Follow the safety instructions to avoid personal injury and property damage. Also, the valid safety instructions for workplaces must be followed.

- Only connect the unit to a power socket with an earthing contact (PE – protective earth)!
- The power supply plug serves as a safe disconnecting device from the line and must always be easily accessible.
- Place the unit on an even surface on a base made of nonflammable material.
- Do not stay in the area below the unit.
- Make sure you read and understand all instructions and safety precautions listed in this manual before installing or operating your unit.
- Set the excess temperature safety installation at least 25 °C below the fire point of the bath fluid.
- Observe the limited working temperature range when using plastic bath tanks.
- Never operate the unit without bath fluid in the bath.
- Pay attention to the thermal expansion of bath oil during heating to avoid overflowing of the fluid.
- Prevent water from entering the hot bath oil.
- Do not drain the bath fluid while it is hot!
  Check the temperature of the bath fluid prior to draining (e.g., by switching the unit on for a short moment).
- Use suitable connecting tubing.
- Avoid sharp bends in the tubing, and maintain a sufficient distance from surrounding walls.
- Make sure that the tubing is securely attached.
- Regularly check the tubing for material defects (e.g., for cracks).
- Never operate damaged or leaking units.
- Always turn off the unit and disconnect the mains cable from the power source before performing any service or maintenance procedures, or before moving the unit.
- Always turn off the unit and disconnect the mains cable from the power source before cleaning the unit.
- Always empty the bath before moving the unit.
- Transport the unit with care.
- Sudden jolts or drops may cause damage in the interior of the unit.
- Observe all warning labels.
- Never remove warning labels.
- Never operate units with damaged mains power cables.
- Repairs are to be carried out only by qualified service personnel.

➢ Some parts of the bath tank and the pump connections may become extremely hot during continuous operation. Therefore, exercise particular caution when touching these parts.

Caution:

The temperature controlling i.e. of fluids in a reactor constitutes normal circulator practice.

We do not know which substances are contained within these vessels.
Many substances are:

- inflammable, easily ignited or explosive
- hazardous to health
- environmentally unsafe

i.e.: **dangerous**

The user alone is responsible for the handling of these substances!
The following questions shall help to recognize possible dangers and to reduce the risks to a minimum.

- Are all tubes and electrical cables connected and installed?
  Note:
  sharp edges, hot surfaces in operation, moving machine parts, etc.
- Do dangerous steams or gases arise when heating?
  Is an exhaust needed when working?
- What to do when a dangerous substance was spilled on or in the unit?
  Before starting to work, obtain information concerning the substance and determine the method of decontamination.

Notice: Check the safety installations at least twice a year!

- Excess temperature protection according to IEC 61010-2-010.
  With a screwdriver turn back the adjustable excess temperature protection until the shut-down point (actual temperature).
- Low level protection according to IEC 61010-2-010.
  To check the function of the float, it can be manually lowered with a screwdriver for example.

4. Operating controls and functional elements

Front view

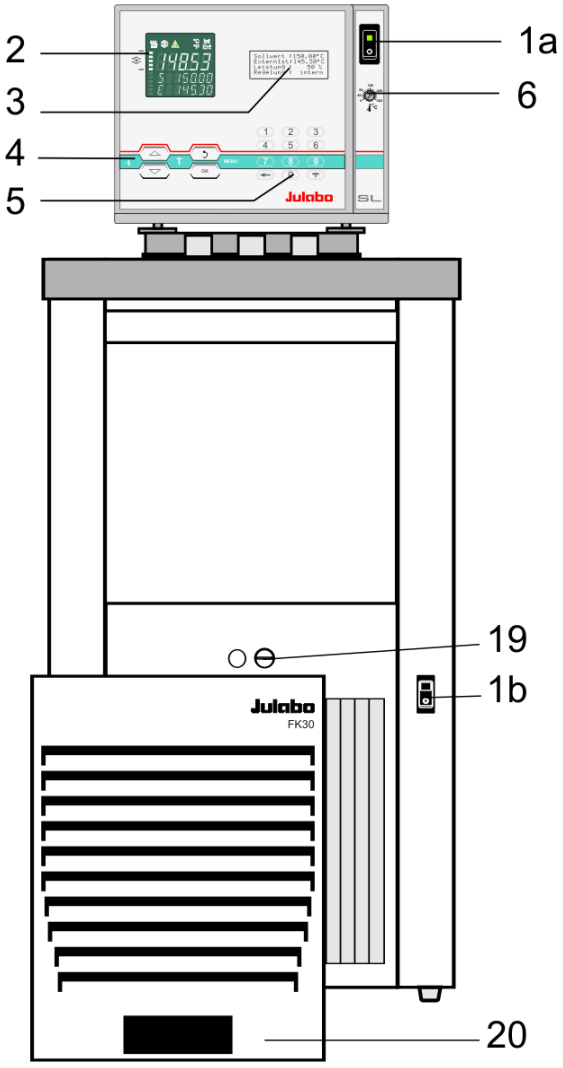

Rear view

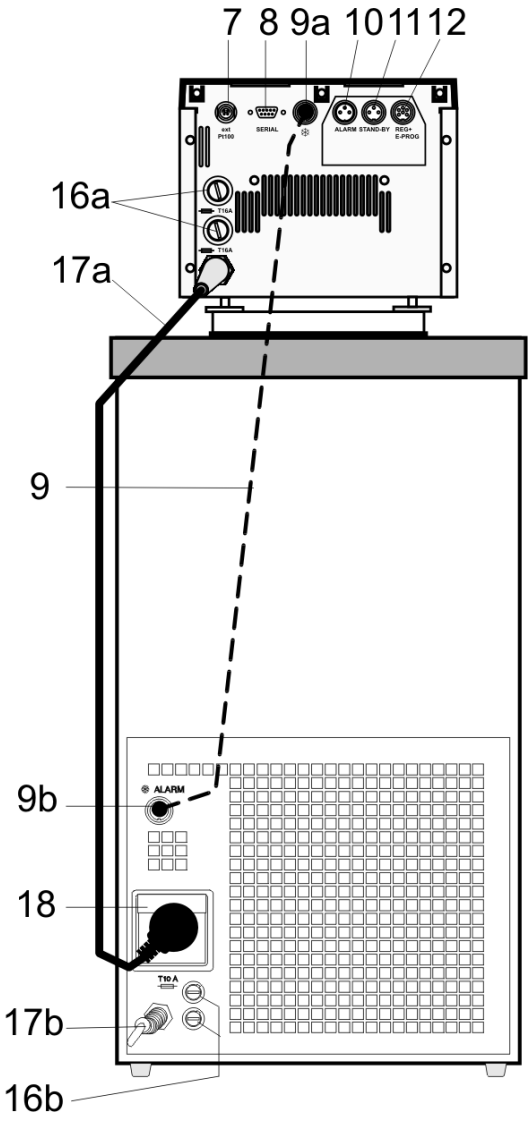

1a  Mains power switch, illuminated for circulator

1b Mains power switch, illuminated for cooling machine

2 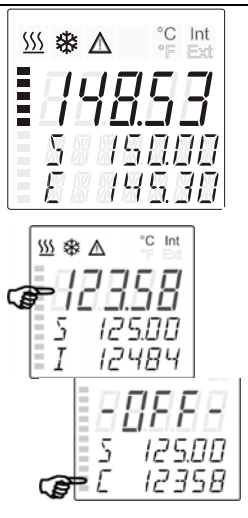

VFD COMFORT-DISPLAY

Header: Control indicators

Line 1: Actual value internal or external
The display is depending on the selected control mode in the menu > Control < (internal or external).
or
Actual value of the precision reference sensor „**C“** xxx.xx

Line 2: Working temp. setpoint, constantly S xxx.xx

Line 3: Actual value (E = external or I = internal or C= reference sensor)
Alternating with the display in line 1

Use the keys ▲ ▼ to indicate further values in line 3

PI Capacity in % - with manipulated variable set to >control<*

PS Capacity in % - with manipulated variable set to >serial<* or >eprog<*
H Heater capacity in Watts
U Mains voltage Volts
F Flow rate in liters/minute
(providing EPROG input set to >Flow rate<)

*refer to >MENU / CONFIGIGURATIO> page 31

2.1

Control indicators in the header:
Heating / Cooling / Alarm /
Remote control

2.2

°C Int
°F Ext

Control indicators in the header:
Temperature indication **Int**ernal or **Ext**ernal actual value
Temperature indication in **°C** or **°F**

2.3



Display for the adjusted pump pressure stage in the -OFF- mode.
Display for the effective pump pressure stage (rotation speed) after start.
Four stages, adjustable via the MENU button, in the menu >PUMP<.

3

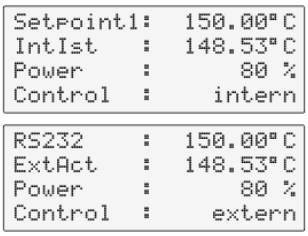

LCD DIALOG-DISPLAY

Line 1: Setpoint and origin of setpoint programming
(Key / RS232 or RS485 / ext. Pt100 / EProg)
Line 2: Actual value - internal or external,
identical to line 1 of the VFD-COMFORT-DISPLAY
Line 3: Heating capacity in %.
Line 4: Control type: internal / external

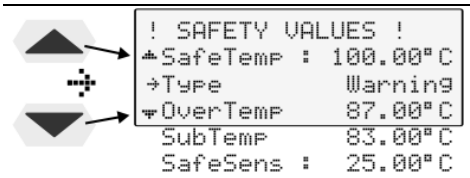

Navigation aid in MENU - Window
Keys ▲ / ▼ :
Selection of menu items / parameters
✣ - Setting in line 3:
Actual value / parameter

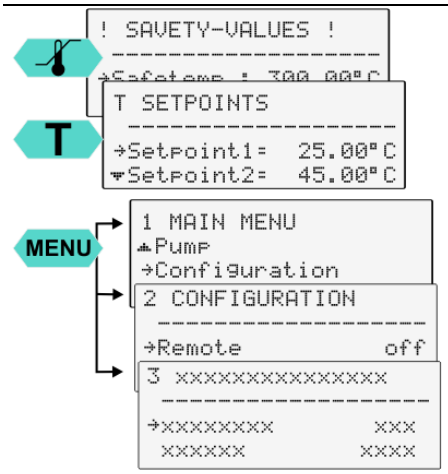

Orientation aid in MENU - Window
Line 1 - name with allocation to key

Safety values
T – Setpoint

MENU

1 Main menu Level 1
2 Submenu Level 2
Example: CONFIGURATION
3 Submenu Level 3

4	Keypad **1**	**Navigation keys**
4.1	OK	1. Key: >OK< Start / Stop (pump / heater) 2. >OK< in the menu Menu item / select submenu for setting Save set value Save selected parameter A beep signals the end of setting
		After the actions Start, Stop and change from VFD Display to standard display the key OK is locked for a short time. The above graph “front side” shows an example for standard display.
4.2		1. Key: >Return< Stop (pump / heater) Special display on VFD Display leave line 3. 2. >Return< in the menu one menu level down Correction function for parameters or values (prior to OK) immediately back to standard display
		OK - icon for „keep key pressed down“.
4.3		1. Key: >Up / Down <temperature – increase/decrease setpoint Push key quickly for single steps, Keep key pressed for fast change. 2. >Up/Down< in the menu selection of menu items / parameters
		Menu keys
4.4		Key: start the menu > warning and safety values<
4.5	T	Key: start the menu >temperature setpoints<
4.6	MENU	Key: display of MENU structure
5	Keypad **2**	
	0 .. 9	Numeric keypad: numerals 0 to 9
		minus / decimal point
		Backspace key on LCD DIALOG-DISPLAY. Setpoint1: 155 °C
6	160 80 240 40 0 320 °C	Adjustable excess temperature protection according to IEC 61010-2-010

Rear view

7	ext Pt100	Socket for external measurement and control sensor or external setpoint programming
8	SERIAL	Interface RS232 / RS485: remote control via personal computer or Socket for a precision reference sensor
9		Socket: control cable of JULABO refrigerated circulator or output for alarm messages

Option: Electronic module		**Order No. 8 900 100**
		The circulator automatically recognizes the connected electronic module.
10	ALARM	Alarm output (for external alarm signal)
11	STAND-BY	Standby input (for external emergency switch-off)
12	REG+E-PROG	Programmer input and temperature recorder output

16a 16b		Mains fuses for Circulator: T16A Mains fuses for cooling machine: T 10,0 A
17a 17b		Mains power cable with plug for circulator Mains power cable with plug cooling machine
18		Built-in mains outlet for connection of circulator (230 V / 16 A)
19		Drain screw with drain connection
20		Venting grid, removable

5. Preparations

5.1. Installation

- Place the unit on an even surface on a pad made of **non-flammable** material.
- Cooling machine, pump motor and electronics produce intrinsic heat that is dissipated via the venting openings! Never cover these openings!
- Keep at least 20 cm of open space on the front and rear venting grids.
- The place of installation should be large enough and provide sufficient air ventilation to ensure the room does not warm up excessively because of the heat the instrument rejects to the environment. (Max. permissible ambient temperature: 40 °C).
  For a fault (leakage) in the refrigeration system, the standard EN 378 prescribes a certain room space to be available for each kg of refrigerant.
  The refrigerant quantity is specified on the type plate.
  > > For 0.25 kg of refrigerant R134a, a room space of 1 m^3 is required.
- Do not set up the unit in the immediate vicinity of heat sources and do not expose to sun light
- Before operating the unit after transport, wait about one hour after setting it up. This will allow any oil that has accumulated laterally during transport to flow back down thus ensuring maximum cooling performance of the compressor.

The bath cover (1) is mounted on the bath tank with 4 captive screws (2).
Required tool: SW3 hexagonal socket wrench with ball-shaped head

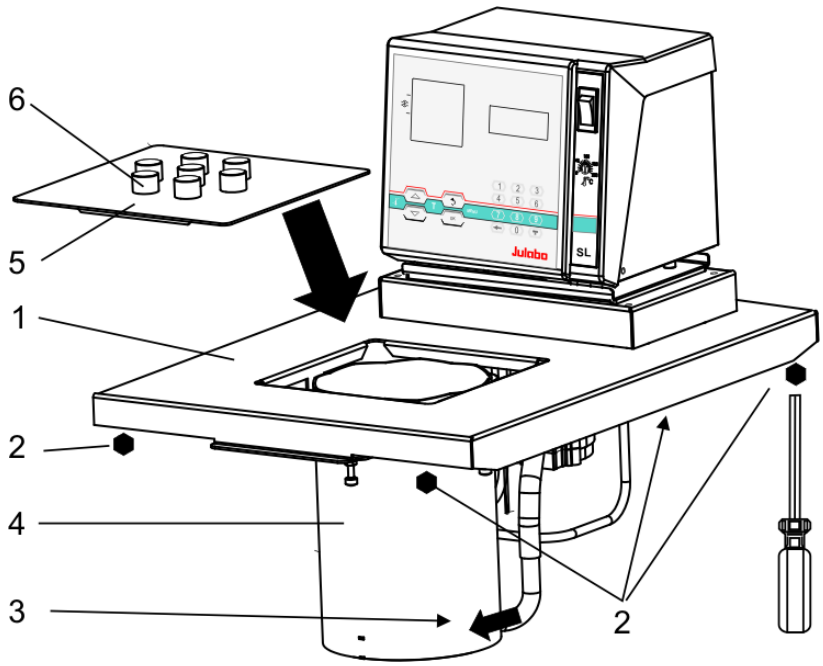

The circulating pump transports the bath fluid to the temperature chamber (4) at the bottom (3). The overflow on top of the chamber ensures a constant fluid level during operation.

The bath cover (5) provides 6 measuring places (6) that can be fitted with different Viton® sleeves..

Order-No.:	Viton® sleeves
8 930 602	2 mm inner dia.
8 930 603	3 mm inner dia.
8 930 604	4 mm inner dia.
8 930 605	5 mm inner dia.
8 930 605	6 mm inner dia.
8 930 608	8 mm inner dia.

ⓘ Take off the complete insert for cleaning. The gasket below the bath cover should be replaced in this case.
Part No.: 7.901.1088 Gasket for bath cover FK30, FK31

5.2. Bath fluids

Caution:
Carefully read the safety data sheet of the bath fluid used, particularly with regard to the fire point!
If a bath fluid with a fire point of ≤65 °C is used, only supervised operation is possible.

Water: The quality of water depends on local conditions.

- Due to the high concentration of lime, hard water is not suitable for temperature control because it leads to calcification in the bath.
- Ferrous water can cause corrosion - even on stainless steel.
- Chloric water can cause pitting corrosion.
- Distilled and deionized water is unsuitable. Their special properties cause corrosion in the bath, even in stainless steel.

Recommended bath fluids:

Bath fluid	Temperature range
soft/decalcified water	5 °C to 80 °C
mixture water/glycol, mixture 1:1	-20°C to 50°C

JULABO bath fluids

JULABO Description		Thermal G	Thermal HY	Thermal H5
Order Number	10 liters	8 940 124	8 940 104	8 940 106
	5 liters	8 940 125	8 940 105	8 940 107
Temperature range	°C	-30 ... 80	-80 ... 55	-50 ...105
Flash point	°C	--	78	124
Fire point	°C	--	80	142
Color		light yellow	clear	clear

JULABO Description		Thermal H10	Thermal H20S
Order Number	10 liters	8 940 114	8 940 108
	5 liters	8 940 115	8 940 109
Temperature range	°C	-20 ... 180	0 ... 220
Flash point	°C	190	230
Fire point	°C	216	274
Color		clear	light brown

See website for list of recommended bath fluids.

ATTENTION: The maximum permissible viscosity is 70 mm^2 /s·

Caution:

Fire or other dangers when using bath fluids that are not recommended:
Use only non-acidic and non-corroding bath fluids.
JULABO assumes no liability for damage caused by the selection of an unsuitable bath liquid.
Unsuitable bath fluids are fluids which, e.g.,

- are highly viscous
  (much higher than recommended at the respective working temperature)
- have a low viscosity and have creep characteristics
- have corrosive characteristics or
- tend to crack.
- **No liability for use of other bath fluids!**

5.3. Filling / draining

Notice:

- Pay attention to the thermal expansion of bath oil during heating to avoid overflowing of the liquid.
- Do not drain the bath fluid while it is hot!
  Recommendation: Temperature range 5 °C to 40 °C
  Check the temperature of the bath fluid prior to draining (by switching the unit on for a short moment, for example).
- Store and dispose the used bath fluid according to the laws for environmental protection.

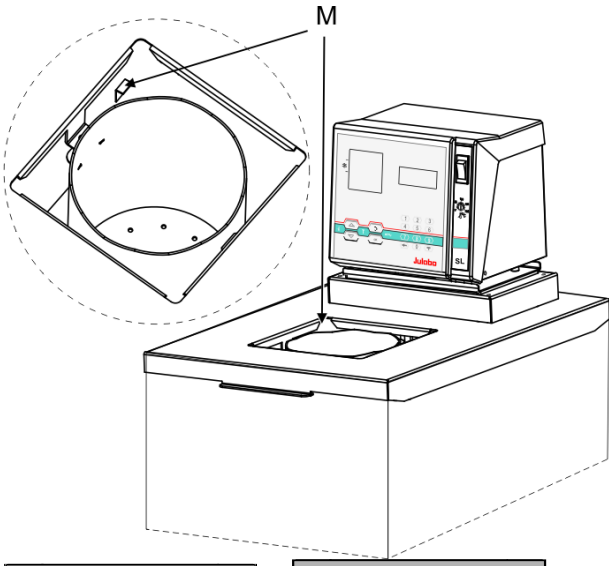

Filling

Take care that no liquid enters the interior of the circulator.

ⓘ The recommended filling level is marked with an angle plate (M) inside the bath.

ⓘ When the filling level does not exceed the marker (M) and providing a suitable bath fluid is used for the specified working temperature range of the unit, neither low liquid level alarm should be triggered nor overflowing of the bath fluid should be caused.

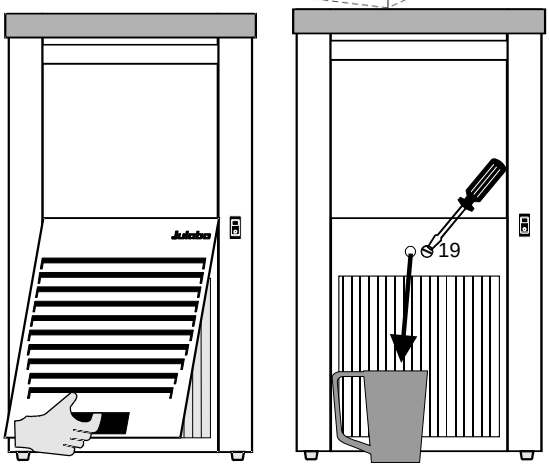

Draining:

- Turn off the unit and disconnect the mains cable from the power source.
- Hold the venting grid, pull out and remove.
- Slide a short piece of tube onto the drain connection and hold it into a container.
- Loosen the drain screw a few turns and drain the unit completely.
- Tighten the drain tap.

6. Operating procedures

6.1. Power connection

Caution:

- Only connect the unit to a power socket with earthing contact (PE – protective earth)!
- The power supply plug serves as safe disconnecting device from the line and must be always easily accessible.
- Never operate equipment with damaged mains power cables.
- Regularly check the mains power cables for material defects (e.g. for cracks).
- We disclaim all liability for damage caused by incorrect line voltages!

Check to make sure that the line voltage matches the supply voltage specified on the identification plate.

- Connect the circulator with mains power cable (17a) to the mains outlet (18).
- Connect the control cable (9) to the ❄ sockets (9a, 9b).
- Connect the refrigerated circulator with mains power cable (17b) to the mains socket.

6.2. Switching on / Selecting the language

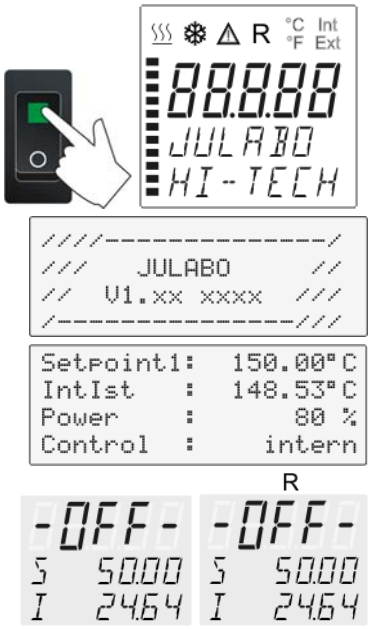

Switching on:

- Turn on the mains power switch (1a).

ⓘ The unit performs a self-test.
Then the software version (example: V 1.12-S008C) appears. The display „**OFF**“ or „**R OFF**“ indicates the unit is ready to operate.

ⓘ The circulator enters the operating mode activated before switching the circulator off:
keypad control mode (manual operation) or
remote control mode (operation via personal computer).

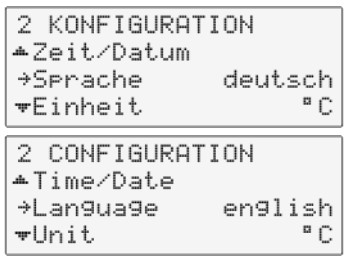

Selecting the language:

There are two options for the language of the LCD DIALOG-DISPLAY: German or English. Select the desired language in the menu >Configuration< under the submenu >Language/Sprache<.

Press the respective keys in the following order:

MENU ➔ ▼ 3x up to menu Configuration OK

▼ 6x up to submenu >Language/Sprache< OK

▼ deutsch / english OK

6.2.1. Switching on the cooling machine

- Switch on the cooling machine using the switch (1b) .

ⓘ Control of the cooling machine:

With the mains switch (1b) turned on, the circulator automatically switches the cooling machine off and on.

To save energy, turn off the cooling machine with the mains switch (1b) whenever cooling is not required.

6.3. Start - Stop

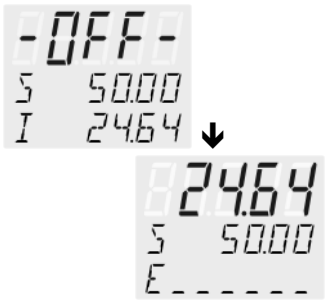

Start:

- Press OK key.
  The actual bath temperature is displayed on the VFD COMFORT-DISPLAY. The circulating pump starts with a slight delay.

Stop:

- Press OK key.
  or
  Keep ↺ 🕑 key pressed.
  The VFD COMFORT-DISPLAY indicates the message "OFF".

6.4. Adjusting the temperature chamber

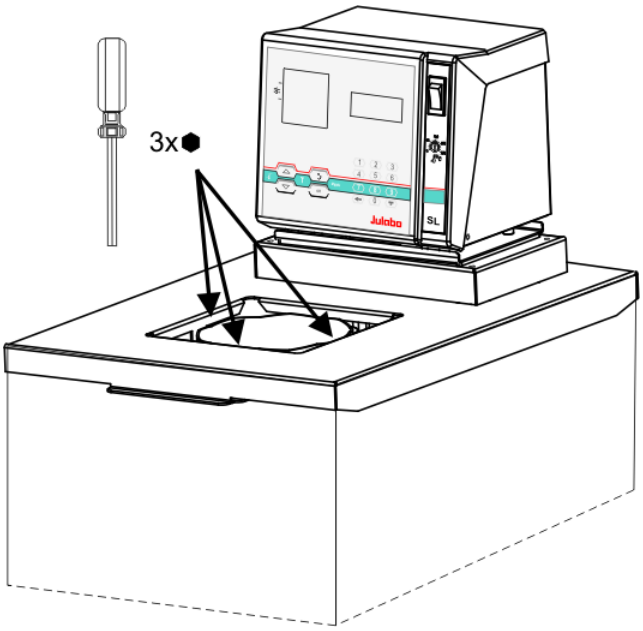

Adjusting the temperature chamber after set up:

- If bath fluid overflow in the temperature chamber is not equal in every direction, an adjustment can be made with the 3 screws that are accessible from above.

  Required tool: SW3 hexagonal socket wrench with ball-shaped head

7. T Setting of temperatures

Press the T key to call up the menu for temperature selection.

3 different working temperatures can be adjusted. Their values are freely selectable within the operating temperature range.

ⓘ The temperatures can be set in start or stop mode.

Setting of working temperature in the T menu

1. Press the key T. The value flashes
2. Select SETPOINT 1 or 2 or 3 using the key ▼ or ▲ .
3. Confirm by pressing the OK key.

ⓘ The circulator uses the new working temperature value for temperature control.

Factory settings:

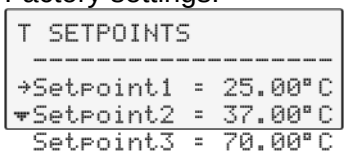

Example:
Adjustment/modification of the pre-setting of "SETPOINT 3"

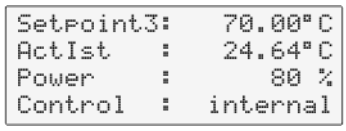

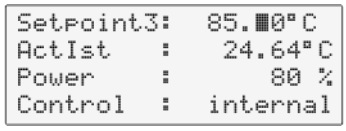

ⓘ If the active Setpoint is changed, the new value is immediately used for the control of the working temperature.
The heater control indicator flashes.

Setpoint3: Change the value from 70.00°C to 80.00°C.
See standard display line 1

- Use the numeric keypad to enter 8 and 5 .
  Then press enter OK to store the value.

Notice: Refer to SETPOINT MAX / MIN in chapter „LIMITS“

8. Safety installations, warning functions

Check the safety installations at least twice a year! Refer to page 14.

Settings for the excess temperature protection > SafeTemp< and for the warning functions > OverTemp< and > SubTemp< are made in a menu which is called up by pressing the key .

Menu item > Type< allows choosing between a warning and an alarm cut-off for the menu items > OverTemp< and > SubTemp<.

Warning:

The excess temperature protection **must** be set at least 25 °C below the fire point of the bath fluid used!
In case of wrong setting there is a fire hazard!
We disclaim all liability for damage caused by wrong settings!

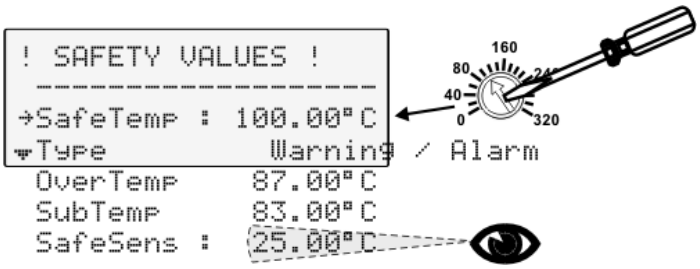

SafeTemp:

Setting range: 20 °C ... 320 °C

ⓘ Rough setting can be effected by using the temperature scale.

Settings:

- Press the key and by pressing the key or select the menu item and confirm the by pressing the key OK.

For setting proceed as follows.

SafeTemp:

- Set the new cut-out value within 30 seconds with a screw driver. Exact display and setting on LCD display
  Recommendation:
  Set over temperature-protective setting >SafeTemp< 5 °C to 10 °C above the set point of the working temperature.

Type:

Switch-over from warning to shutdown function

- Change the parameter by pressing the key and confirm by pressing the key OK.
  or
  pressing the key if the parameter is to be retained.

Possible parameters: **warning or alarm**

OverTemp :

SubTemp:

- Set value on numeric keypad and confirm by pressing OK

Example: 83.00 °C

Press the keys 8 and 3 and confirm by pressing OK

Sensor:

Indicated is the temperature value of the safety sensor.

SafeTemperature:

Setting range: 20 °C ... 320 °C

Indicated is the cut-out value set with a screwdriver on the excess temperature protection device.

This safety installation is independent of the control circuit. When the temperature of the bath fluid has reached the safety temperature, a

complete shutdown of the heater and pump is effected.

The alarm is indicated by optical and audible signals (continuous tone).
The following error message appears on the VFD COMFORT-DISPLAY:

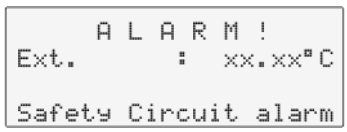

Press **OK** for help on the LCD ↓

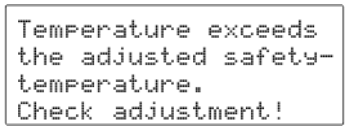

ⓘ Depending on the setting of >ControlType - internal or external< the actual temperature values for both sensors are shown/indicated on both displays.
Examples: I 94.06 and Ext. : xx.xx°C

Type: >Warning< or >Alarm<
For the two menu items >OverTemp< and >SubTemp< choose between a warning message being signaled or a complete shutdown of the main functional elements such as heater and circulating pump being effected.

OverTemperature**:** **SubTemp**erature**:**
If for a sensitive temperature application task adherence to a working temperature value >Setpoint< is to be supervised, then set high and low temperature warning values.
In the example below, the >Setpoint< of 85 °C is surrounded by the values >OverTemp< 87 °C and >SubTemp< 83 °C. The electronics immediately registers when the actual temperature attains a temperature out of the limits and it follows a reaction according to what is set in the menu item >-Type<.

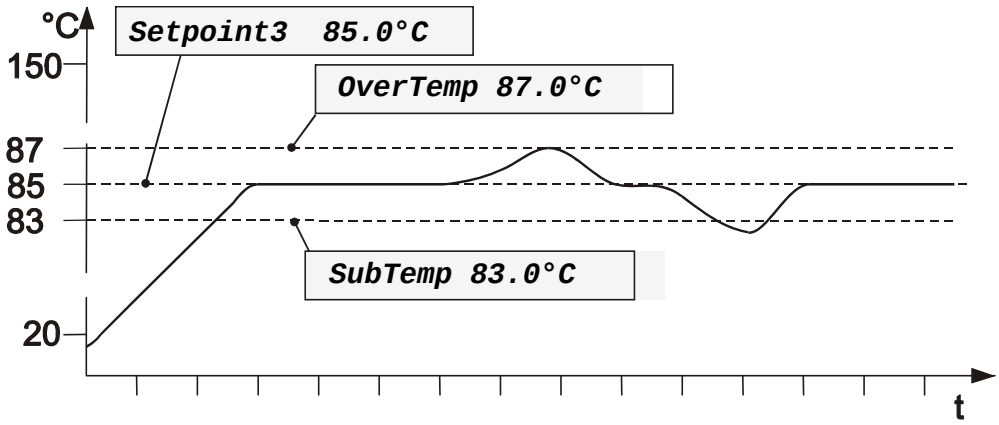

ⓘ The warning functions are only triggered when the actual bath temperature, after start from the „OFF“ or „rOFF“ mode, lies within the set limits for 3 seconds.

- Setting >**WARNING**<
  A mere warning function with optical and audible warning signal (interval tone) A message appears on the VFD COMFORT-DISPLAY:

or

OverTemp SubTemp

The LCD –DISPLAY shows the message:

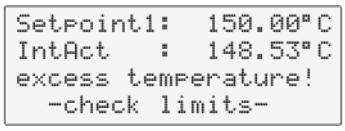

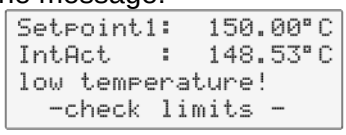

- Setting >**ALARM**<
  Temperature limit with shutdown of heater and circulating pump.
  An audible alarm sounds (continuous tone) and a message appears on the VFD COMFORT-DISPLAY:

or

OverTemp SubTemp

The LCD -DISPLAY shows the message

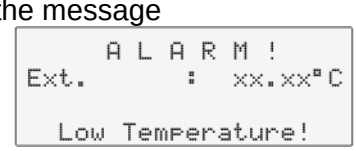

Press **OK** for help on the LCD

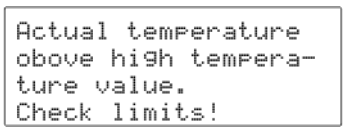

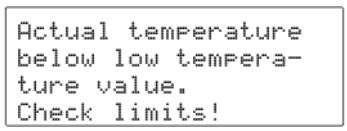

8.0.1. Early warning system, low level protection



DBGM: 20306059.8

This low level protection is independent of the control circuit and is divided into two sections:

1. Switch in stage 1 recognizes a critical fluid level 😐.
   An audible warning (interval tone) sounds and a message appears on the VFD COMFORT-DISPLAY.

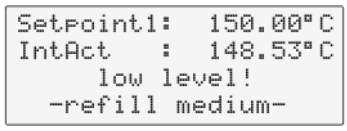

Refill bath fluid!

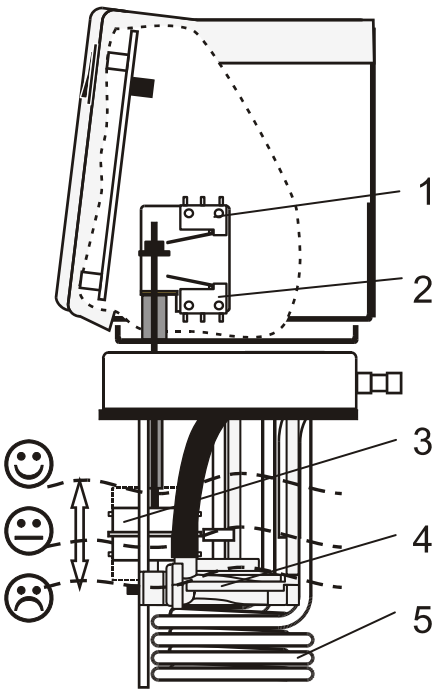

2. Switch in stage 2 recognizes a low fluid level ☹.
   If stage 2 of the low level protection device (according to IEC 61010-2-010) is triggered, a complete shutdown of the heater and circulating pump is effected.
   A continuous alarm tone sounds and a message >ALARM< >CODE 01< appears on the VFD COMFORT-DISPLAY.

Press **OK** for help on the LCD ↓

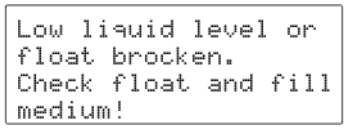

Turn off the unit with the mains switch, refill bath fluid and turn the unit on again!

3. Float
4. Circulating pump
5. Heater

Warning:

For refill always use the same bath fluid type that is already in the bath.
Bath oils must not contain any water contaminants and should be pre-heated to the actual bath temperature! Explosion hazard at higher temperatures!

9. MENU Menu functions

MENU

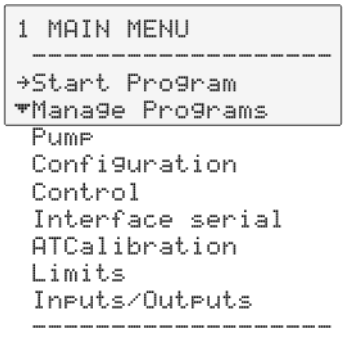

The term „menu functions“ refers to adjustments such as

Menu level 1

	Start program This menu will start a previously set program.	Page 31
	Administration and creation of programs	Page 36
	Electronically adjustable pump capacity The capacity of the circulating pump is set by adjusting the motor speed.	Page 40
	• Configuration of the unit Remote – on / off (remote control via RS232) Setpoint ext - Switch over external setpoint setting Autostart – AUTOSTART on / off Off-Mode – Pump on / off ACTVAR - Switch over input variable Time / Date – setting time and date Language – english / deutsch Unit – Temperature values can be displayed in °C or °F. Program Type – Time or Gradient (grad) Reset – factory settings C-Sensor (Precision Pt100 reference sensor)	Page 41
	Control characteristics and parameters ControlType - Control internal or external Selftuning Dynamic - internal CoSpeed – external Control parameters - XP-, TN-, TV- internal Control parameters - XP-, TN-, TV- XPU-, external	Page 49

Menu level 1

	Adjustable interface parameters BAUDRATE, PARITY, HANDSHAKE	Page 55
	ATC - Absolute Temperature Calibration, Sensor calibration internal sensor, Sensor calibration external sensor 3-point calibration	Page 56
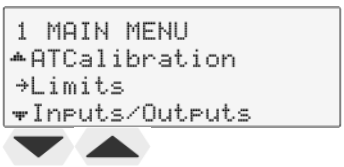	Limitations of temperature and capacity Setpoint Max / Min - Maximum and minimum setpoint Heating Max – Set maximum heating Cooling Max – Set maximum cooling Internal Max / Min – Limitation of the temperature range Upper band / Lower band – Band limit	Page 63
	Analog inputs/outputs Recorder output – CHANNEL 1, 2, 3 EPROG – External programmer input Ext-StBy - Stand-By input ALARM - output	Page 65

9.1. Start of a program

The start menu of the integrated programmer allows one of six previously stored temperature programs to be called up and started. The profiles are started manually or via the integrated timer.

ⓘ Requirements:

1. Create a program. (refer to next chapter)
2. Return to the Start-MENU and confirm the desired setting of each MENU item with the key OK
3. Set a start time (>TIME< >DATE< >YEAR<) if the program is to be started by the internal timer.

>Program Number<	Select the program that should be started. 0 ... 5
> at Step<	Select the Step at which the program should be started. 0 … 59
> Runs <	Select the number of program repetitions. 1 ... 99
> Program End<	Status at program end . StdBy, PSetp, Setp 1, Setp 2, Setp 3
> RUN <	Start time (now / time)

MENU

OK

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Parameter /Value	
		• Set a parameter using the numeric keypad and confirm by pressing OK . Possible parameters: 0 …5
		• Set a parameter using the numeric keypad and confirm by pressing OK . Possible parameters: 0 … 59
		• Set a parameter using the numeric keypad and confirm by pressing OK . Possible parameters: 1 … 99
		• Set desired parameters with ▲ ▼ and OK . Possible parameters: StdBy , PSetp, Setp 1, Setp 2 , Setp 3

Level 2	Parameter /Value	
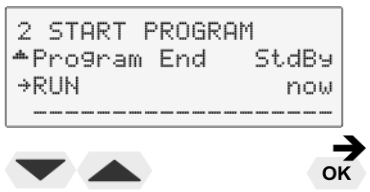	 or 	• Set desired parameters with ▲ ▼ and OK . Confirm >now< with the OK key and the program will start immediately **or** start at the set time under parameter (time). Set time in the example below: 09. August 2009, 11:15 hrs
Submenu TIMER 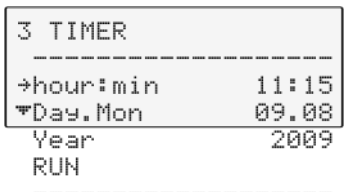		If the parameter **time** is selected, a further submenu opens for setting the start time. Set the time for the start of the program in the submenu >3 TIMER<.
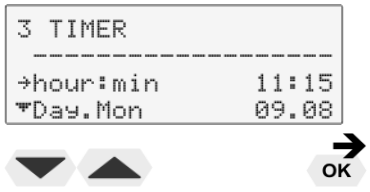		• Set starting time using the numeric keypad and confirm by pressing OK . Example: (hh:mm) 1 1 - 1 5 + OK
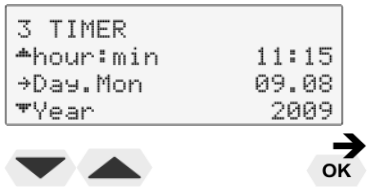		• Set day and month using the numeric keypad and confirm by pressing OK . Example: (TT/MM) 0 9 - 0 8 + OK
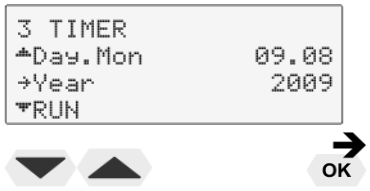		• Set year using the numeric keypad and confirm by pressing OK . Example: (JJJJ) 2 0 0 9 + OK
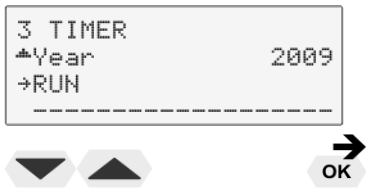		Confirm >Starten/Start?< by pressing OK and the program starts at the set time.
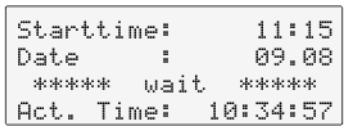	Display of waiting time until start: The unit switches to waiting mode and a flashing line “wait” appears on the LCD DIALOG-DISPLAY. The start time and current time are permanently indicated on the display. It might be necessary to check the correct setting of the internal real time clock (see MENU configuration)	

9.1.1. Status at the end of a program

```
Setpoint3:   80.00°C
IntAct    :   80.00°C
Power     :       3 %
Control   :  internal
```

```
T SETPOINTS
↑Setpoint1 = 25.00°C
→Setpoint2 = 58.00°C
↓Setpoint3 = 85.00°C
```

```
Setpoint2:   58.00°C
IntAct    :   60.00°C
Power     :       0 %
Control   :    intern
```

Program end **StdBy , PSetp, Setp 1, Setp 2 , Setp 3**

This parameter is used to determine if the unit switches to the -OFF- condition at the end of a profile or if temperature control is continued, and the working temperature setpoint that is to be used if temperature control is continued.

StdBy – If the end of the profile is reached, the circulator switches to the -OFF- condition. The VFD display indicates the working temperature setpoint that was displayed in line 2 before the program was started (example: S 25.00 °C).

PSetp –(Setpoint of the **P**ro**G**rammer) At the end of the program, the setpoint of the last program step is written to the position of setpoint 3 (example: 80.00 °C) and indicated in line 1 of the LCD display. The circulator operates and controls to this temperature until the key OK is pressed or a new profile is started.

Setp 1, Setp 2, Setp 3 – ("**Setp**" short for **Setpoint**)
Before starting the programmer, a temperature value is set for one of the three setpoints in the T menu.
(example: setpoint 2 58.00 °C)
The circulator operates and controls to this temperature at the end of the profile until the key OK is pressed or a new program is started.

9.1.2. Indication after successful start

The started programmer displays the currently calculated setpoint in line 1. The value changes until the final temperature of the section is reached (temperature ramp).

1st line: Setpoint of the programmer

2nd line: Actual temperature value
for **internal control** = IntAct: xxx.xx
for **external control** = ExtAct: xxx.xx

3rd line: Selected profile and the current section (step).

4th line: With the ▼ ▲ keys, the following information can be displayed in line 4.

- Remaining time of the current section (standard display)
- Total remaining time: profile x number of repetitions (**`All: Days/hours:minutes:seconds`**)

Particularities :

1. If a total time of more than 999 days is calculated, only the hours are displayed by the unit. (**`All: hours:minutes:seconds`**)
2. If the time period of a section is edited after the start, then the remaining total time can no longer be displayed.

Examples:

```
Set     :     XX.XX°C
IntAct  :     XX.XX°C
ProgNr.:2   Step:  2
Remain  :   03:32:25
```

```
Set     :     XX.XX°C
IntAct  :     XX.XX°C
ProgNr.:2   Step:  2
All     :ttt/hh:mm:ss
```

9.1.3. Editing after Start

The programmer allows a running program to be edited.

Initiation and exit of the editing function:

- After the start enter the submenu „3 EDITOR“.by pressing the key MENU
  See chapter „program administration, creation“ page 36
- Exit the editing modus anytime by pressing the key ↩ .

Particularity for changes in a section that is currently in process.

ⓘ If the target temperature is changed, the slope of the ramp is automatically calculated based on the remaining time of the section.

ⓘ If the time period is changed, the slope of the ramp is automatically calculated based on the new total time of the section.

ⓘ The “remaining total time” (profile x number of repetitions) as described on page 33 can no longer be displayed.

9.1.4. Interrupting a program

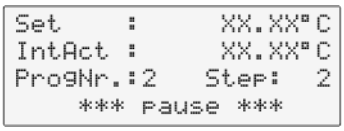

ⓘ Press the ↩ key to interrupt or continue a profile.
The setpoint and time period set for the corresponding section are thus stopped at the values presently achieved.
The instrument is put on hold and the message “pause” flashes on the LCD DIALOG DISPLAY.



ⓘ A program can be interrupted or restarted by an external shut-off.

Important:
For this, in the >**Inputs/Outputs**< menu, the menu item >**Ext. StBy**< must be set to >**active<**
and in the >**Configuration**< menu, >**Autostart<** needs to be set

ⓘ Setpoint control and timer are interrupted by breaking the contact “AK”.
The instrument is put on hold and the message “Stand-By” flashes on the LCD DIALOG-DISPLAY.

⚠ **Notice**: **This is not an actual emergency switch-off.**

Warning:
Following a power interruption, it would be possible in this condition for the instrument to restart automatically. The safety and warning functions of the instrument should always be used to their fullest capacity.
Refer to **Warning** page 45.

9.1.5. Interruption after a power failure

It is possible to operate the programmer safely in case of a power failure.
Important:
For this, >**Autostart<** needs to be set in the >**Configuration**< menu.

ⓘ If the AUTOSTART function is activated, the programmer starts again at a point approx. 20 seconds before the interruption took place. However, an uncontrolled change of the bath temperature has occurred.

ⓘ Power failure when the instrument is on hold if start is effected via the built-in timer:
If the starting time is not yet reached, the programmer is put on hold again.
If the starting time is exceeded, the programmer starts immediately.

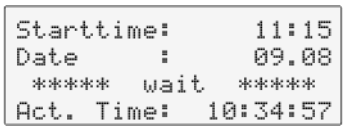

9.1.6. Termination of a program

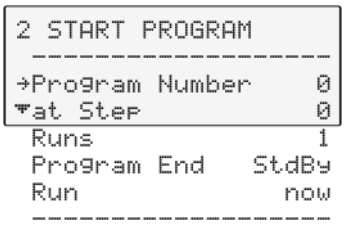

ⓘ A program can be terminated by pressing . The programmer switches back to the Start menu.

Further procedures are defined in the MENU >START PROGRAM<, menu item >Program End <.

Example: >Program End - StdBy<



The VFD COMFORT-DISPLAY displays “OFF”.

Interruption after a power failure

In case of a power failure, the reaction of the circulator is the same as when switched off and on again with the mains switch.

The VFD COMFORT-DISPLAY displays “OFF”.

9.2. Program administration, creation

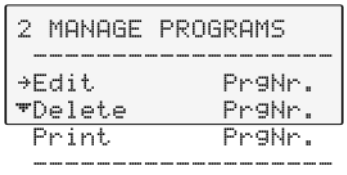

The integrated programmer permits fast and easy programming of setpoint temperature sequences. This temperature sequence is called program. A program is composed of individual sections (Step).
The sections are defined by duration (t) or Gradient (°/t) and target temperature. The target temperature is the setpoint (SP), which is achieved at the end of a section. The programmer calculates the temperature ramp from the difference in time and temperature.

Create programs

A flashing segment indicates that a number needs to be entered.
Under the submenu “Edit”, enter a program number.
Six programs may be stored (numbers 0 to 5).

When the program is running, only sections with complete information for the target temperature and time period are considered.
It makes sense to skip section numbers in the profile in order to use them later for corrections to the profile.

Important:
If a time of 00:00 is set for a profile, the profile is continued with the next section only after the setpoint temperature (±0.2 °C) is reached.

Example:

Step	(Nr.)	1	3	5	6	9	11	14
Setpoint	(°C)	50	50	100	100	80	80	20
Time	(h:m)	00:08	00.02	00:10	01:05	00:10	00:05	00:30

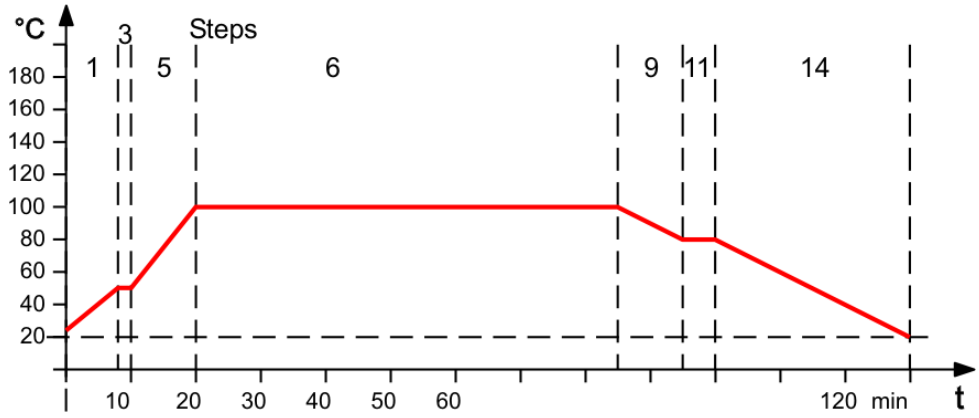

Editing

MENU

OK

PrgNr:	Set the program you wish to create. 0 ... 5
SP:	Setpoint
TI :	Time [hh:mm] or
GRD:	Gradient [°/t] = [°/min] Change type of program in MENU >configuration<, menu item >Programmtyp/program type< .
ST:	Step 0 … 59

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	
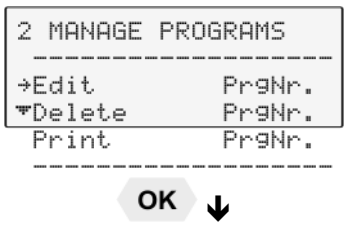 OK	Example: Program (PrgNr.) 2 is to have a target temperature with a set point (SW) of 100.00 °C in section t (ABS) 3. Duration (ZI) 1 hour.
	Select the program number. • Set the desired >PrgNr.< by pressing ▲ ▼ and OK .
Level 3	ⓘ For the selected section >ST< a setpoint >SP< and the duration >TI< or the gradient >GRD< are entered in the right half of the input window.
 or 	Input window for >ST<, >SP< and >TI< / >GRD< **1.** Set the desired Step >ST < by pressing ▲ ▼ and OK . **2.** Set set point >SP< by using the numeric keypad and confirm by pressing OK . **3.** Set the time >TI< or a gradient >GRD< using the numeric keypad and confirm by pressing OK .
	ⓘ By confirming time or GRD the values on the left side of the input window are moved. • The values for the next section are entered in the right half of the input window. See above **1. / 2. / 3.**

Delete

It is possible to delete an entire program or consecutive sections

Delete PrgNr: Set the program you wish to delete
0 ... 5

Delete from Step X to Step X (0 … 59)

MENU

OK

Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Submenu >Delete<
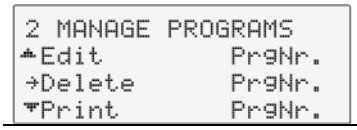	• Set menu item >Delete PrgNr.< by pressing ▼ and OK.
	• Set desired PrgNr with ▲ ▼ and OK. Example: PrgNr. 0
Level 3	Input window: delete sections.
   	• Select menu items >from Step< and >to Step< one after the other by pressing ▼ and OK. • Select the desired section for every menu item by using the numeric keypad and confirm by pressing OK. Example: >from 0< >to 59< • Select menu item >delete< by pressing ▼ and OK
	• Confirm >Delete?< by pressing OK.
	ⓘ The delete procedure is confirm by indication of the message >delete< on the LCD display.

MENU

OK

Print

Every program can be printed via the serial interface for control and documentation purposes.

ⓘ Press the key if a parameter is to be retained. (prior to OK)

Level 2	Submenu >Print<
	• Set menu item >Print PrgNr.< by pressing ▼ and OK.
	• Set desired >PrgNr.< by pressing ▲ ▼ and OK. Example: 4
Level 3	
	• Confirm ✣ > Print< by pressing OK.
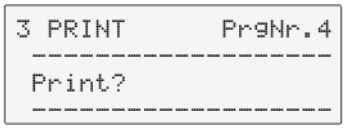	• Confirm >Print?< by pressing OK.
 	ⓘ Printing and end of printing are confirmed by successive messages on the LCD display as shown on the left.

9.3. Setting the pump pressure

MENU

OK

The capacity of the circulating pump is set by adjusting the motor speed

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Submenu >Pump<
	The set pump stage is displayed. Example: 1 • Confirm by pressing OK.
	• Set required pump stage by pressing ▲ ▼ and OK. Example: 3

Example:

Adjusted Effective

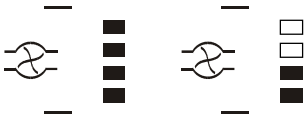

Adjustable pump capacity stage 1 ... 4

Illuminated display: for pump pressure

ⓘ Indication of the adjusted pump pressure stage in the –OFF- mode.

ⓘ Indication of the effective pump pressure stage (rotational speed) after start.

To protect the pump motor, the rotational speed changes with the load applied, for example, depending on the viscosity of the bath fluid at different working temperatures.

Flow rate: 22 ... 26 l/min

Pump capacity stage		1	2	3	4
Pump pressure	[bar]	0.4	0.5	0.6	0.7
Suction pump	[bar]	0.2	0.26	0.33	0.4
Total capacity in a loop circuit	[bar]	0.6	0.76	0.93	1.1

9.4. Configuration

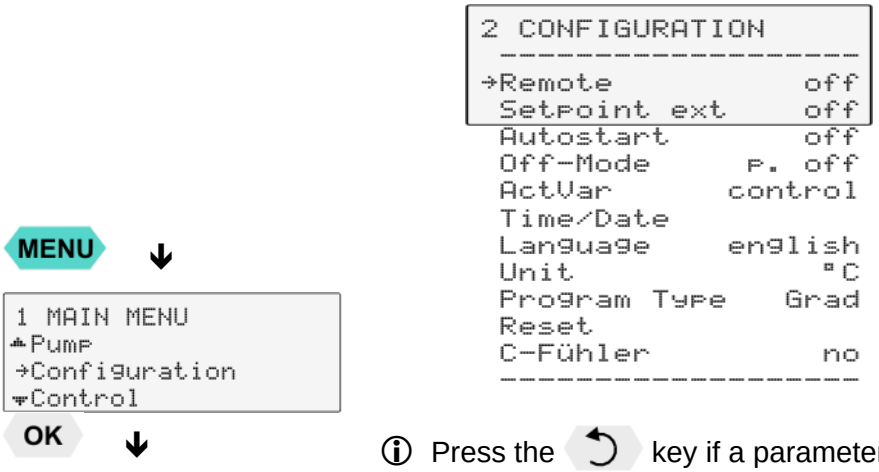

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Parameter level	
2 CONFIGURATION →Remote off Setpoint ext off OK ▼▲	2 CONFIGURATION Remote (RS232) off or 2 CONFIGURATION Remote (RS485) off	Remote control via serial interface. Possible parameters: **off / on** ⓘ Switch on and off remote control by pressing ▲ ▼ and OK ⓘ First set the >type< of interface (RS232 or RS485) in the MENU >INTERFACE SERIAL< and then switch >Remote< to >on<. ⓘ Control display in the top line R for Remote ⓘ ○ ○ Connect SERIAL with PC.
2 CONFIGURATION Remote off →Setpoint ext off Autostart off OK ▼▲	2 CONFIGURATION Setpoint ext off • Switch over setpoint setting by pressing ▲ ▼ and OK	External setpoint setting Possible parameters: **off / Eprog / PT100** • Switch over setpoint setting by pressing ▲ ▼ and OK off – Setpoint setting with the keys or Setpoint setting via the analog socket „ext. Pt100 or analog socket >REG+EPROG<
2 CONFIGURATION Setpoint ext off →Autostart off Off-Mode p. off OK ▼▲	2 CONFIGURATION Autostart off	Autostart Possible parameters: **on / off** • Switch on and off Autostart by pressing ▲ ▼ and OK

Level 2	Parameter level	
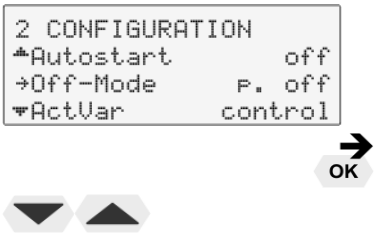		Pump-Mode Possible parameters: **P. on / P. off** • Switch on and off >Off-Mode by pressing ▲ ▼ and OK P.on continuous operation of circulating pump P.off circulating pump is linked to Start/Stop
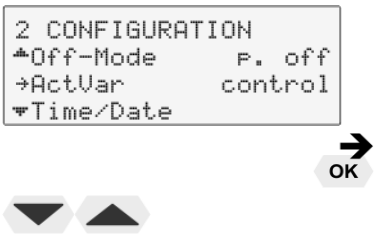		ActVar **-** actuating variable Possible parameters: **control, Eprog, serial** ⓘ Set desired parameters with ▲ ▼ and OK. ⓘ Programming of variables for the parameters > **serial** < or > EPROG < is only accepted, if the unit is in Start mode
		Time, Date, Year see next page
		Language Possible parameters: **deutsch / english** • Set desired parameters with ▲ ▼ and OK.
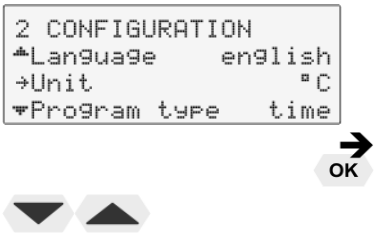		Unit Possible parameters: **°C / °F** • Set desired parameters with ▲ ▼ and OK.
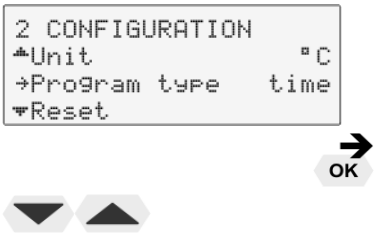		Program type Possible parameters: **time / grad** • Set desired parameters with ▲ ▼ and OK.

Level 2	Parameter level	
2 CONFIGURATION Program type time Reset OK ▼ ▲	2 CONFIGURATION Reset? 2 CONFIGURATION Reset: Running...	Reset • Return to factory settings by pressing OK ⓘ >Reset?< returns all set values to the factory setting except for date and time. ⓘ A RESET can be effected only in the – OFF- mode. ⓘ During the message >Running < all parameters are reset to factory settings.
2 CONFIGURATION Reset C-Sensor yes OK	2 CONFIGURATION C-Sensor ⇳ yes	C-Sensor (Precision Pt100 reference sensor) Possible parameters: **yes / no** • Set desired parameters with ▲ ▼ and OK.

Level 2	Level 3	Parameter / Value
2 CONFIGURATION ActVar control Time/Date Language english OK	3 SET TIME/DATE hour:min 11:50 Day.Mon 07.07 OK ▲ ▼ 3 SET TIME/DATE hour:min 11:50 Day.Mon 07.07 Year 2009 OK ▲ ▼ 3 SET TIME/DATE Day.Mon 07.07 Year 2009 CURRENT: 12:05:16 OK ▲ ▼ 3 SET TIME/DATE Year 2009 CURRENT: 12:05:16 OK	Possible parameters: Time >hour:min Date >Day:Mon Year • Succesively set time, date and year using the numeric keypad and confirm by pressing OK. 3 SET TIME/DATE hour:min 11:50 Example: 1 1 ∓ 5 0 OK 3 SET TIME/DATE Day.Mon 07.07 3 SET TIME/DATE Year 2009 Only the actual time is displayed. 3 SET TIME/DATE CURRENT: 12:05:16

The internal real time clock allows starting a program any time. The clock is set to the local mean time (MEZ) at the factory.

ⓘ If the unit is operated in a different time zone, the clock can be adjusted in this menu.

ⓘ Change summer/winter time in this menu

9.4.1. Remote control via the serial interface

Factory setting: off

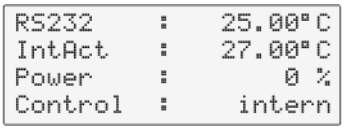

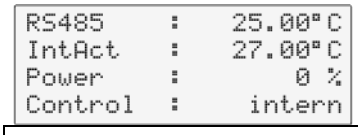

Setpoint is set via the serial RS232/RS485 interface through a PC or superordinated data system.

In the header of the VFD COMFORT-DISPLAY, an "**R**" illuminates. It indicates that remote control mode is active.

➔ The selected setting is shown on the LCD DIALOG-DISPLAY.

IMPORTANT: additional measures for remote control

ⓘ RS232 or RS485:
First set >type< of interface in the MAIN MENU > Interface serial < the switch >Remote< to >on<.

ⓘ Connect the circulator to the PC using an interface cable.

ⓘ Check the interface parameters of both interfaces (circulator and PC) and make sure they match.
(See 12.1. Setup for remote control page 80)

9.4.2. Keypad control or setpoint setting via the analog input

Factory setting: off

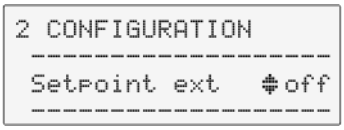

The selected mode is indicated on standard display.

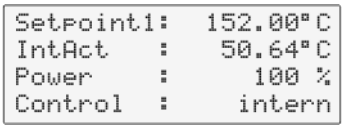

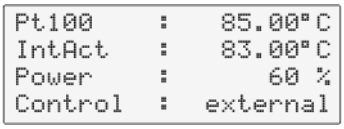

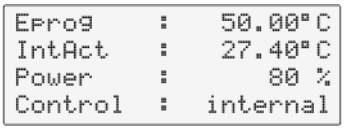

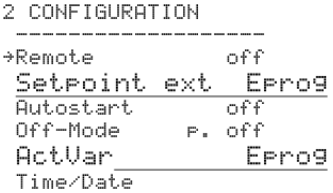

In addition to the serial interface via remote control the circulator offers the possibility to adjust the setpoint via analog interface >ext. Pt100< or >REG+E-PROG<.

Possible parameters:

off - Setpoint is set via the keypad or via the integrated programmer. (factory setting

Pt100 - Setpoint setting via the analog socket „ext. Pt100" using an external temperature sensor or an appropriate voltage/current source.

Eprog - Can only be adjusted when an electronic module with analog connections is used (option).
Setpoint setting via the analog interface REG+E-PROG connection with an external voltage or current source or a programmer.

Important:

ⓘ Connect the external voltage or current source or a programmer to the circulator via the socket REG+E-PROG (see page 70).
In the menu >MENU Inputs/Outputs< set the parameter >Erog-INPUT< and the input variables >Eprog-signal< (see page 70).

ⓘ The E-Prog input can only be used either under menu item >Setpoint ext < or under menu item >ActVar<

9.4.3. Autostart

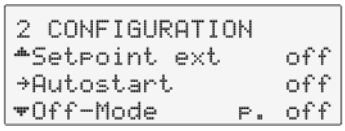

Possible parameters:

on - Autostart on

off - Autostart off (Factory setting)

Note:

The circulator has been configured and delivered by JULABO according to N.A.M.U.R. recommendations. This means for the start mode that the unit must enter a safe operating state after a power failure (non-automatic start mode). This safe operating state is indicated by “**OFF**” or “**R OFF**” on the VFD-COMFORT-DISPLAY. A complete shutdown of the main functional elements such as the heater and circulating pump is effected simultaneously.

The values set on the circulator remain stored, and the unit is returned to operation by pressing the start/stop key (in manual control mode).
In remote control mode, the values need to be resent by the PC via the interface.

Should such a safety standard not be required, the AUTOSTART function (automatic start mode) may be activated, thus allowing the unit to be started directly by pressing the mains power switch or using a timer.

ⓘ The AUTOSTART function can be used only if the setpoint is set via >keyboard<, >eprog<, or >ext. Pt100<.

Warning

For supervised or unsupervised operation with the “AUTOSTART“ function avoid any hazardous situation to persons or property

Take care to fully observe the safety and warning functions of the circulator.

9.4.4. Off-Mode

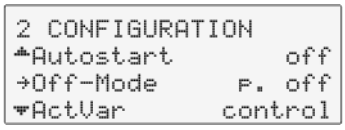

OFF-Mode

Normally the circulating pump is switched via the start/stop signal. However, if circulation should be maintained even in the -off- condition, the parameter >**pump on<** needs to be set.

Possible parameters:

P.on Circulating pump in continuous operation

P.off Circulating pump linked to Start/Stop (factory setting)

9.4.5. ActVar - actuating variable

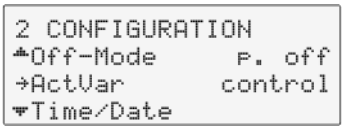

The variable *(ACTuating VARiable)* corresponds to the extent to which the heater or cooling unit of the circulator is controlled. Heat or cold is applied to the bath according to this variable. If this happens with the control electronics of the circulator, called > control < in this particular case, the bath temperature is exactly heated and maintained constant at the adjusted setpoint.

ⓘ Programming of variables for the parameters > SERIAL < or > EPROG < is only accepted, if the unit is in Start mode.







Possible parameters:

control – The internal control electronics of the circulator controls the heater and the connected cooling unit. Self-tuning is possible.. (factory setting)

serial – – The heater or the connected cooling unit receives the control signal via the serial interface. Self-tuning is not possible.

Eprog - The heater or the connected cooling unit receives the control signal via the E-Prog input. Self-tuning is not possible.
- Setting requires electronic module.

Important:
Set the parameter >Eprog< and the input variables also in the menu >Inputs/Outputs< (see page 70).

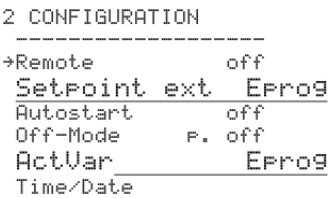

Note:
The E-Prog input can only be used either under menu item >Setpoint ext< or under menu item > ActVar <.

Warning:

The working temperature range of the circulator is determined during configuration. If set to >Control<, this range cannot be exceeded.
If set to > Serial < and > Eprog <, heat or cold is applied to the bath without control. The permissible maximum temperature can be exceeded. The user has to take adequate precautions for temperature control.
Materials, such as gaskets or insulations for example, may be damaged or destroyed, if the permissible maximum temperature is exceeded.

The safety and warning functions > < of the instrument must always be used to their fullest capacity.

9.4.6. Setting of clock and date

The internal real time clock allows starting a program any time. The clock is set to the local mean time (MEZ) at the factory.

ⓘ If the unit is operated in a different time zone, the clock can be adjusted in this menu.

ⓘ Change summer/winter time in this menu

```
2 CONFIGURATION
↑ActVar       control
→Time/Date
↓Language     english
```

9.4.7. Language

There are two options for the language of the LCD DIALOG-DISPLAY: German and English.

```
2 CONFIGURATION
↑Time/Date
→Language     english
↓Unit             °C
```

Possible parameters:

deutsch / english

9.4.8. Unit

Temperature values can be displayed in °C or °F.

With this change, all adjusted temperature values are converted and displayed in the new unit.

```
2 CONFIGURATION
↑Language     english
→Unit             °C
↓Program typ     Zeit
```

Possible parameters:

°C (factory setting)

°F

9.4.9. Program type

A program can be created with the parameters time or gradient.

```
2 CONFIGURATION
↑Unit             °C
→Program typ     time
↓Reset
```

Possible parameters:

time (factory setting)

Grd (Gradient) [°/t] = [°/min]

9.4.10. Reset

A Reset will return all values to factory setting except for date and time.

```
2 CONFIGURATION
↑Program typ     time
→Reset
 ------------------
```

ⓘ A Reset can be effected in the >OFF< mode only.

9.4.11. C-Sensor - Precision reference sensor

Temperature measurement with a precision reference sensor

Factory setting: no

Precision reference sensor for applications in quality assurance, calibration services and laboratories.



SERIAL

Possible parameters:

yes – Temperature measurement with a precision reference sensor

no

- Connect the higly accurate temperature sensor to the RS232 socket (**SERIAL**) on the rear of the circulator.
- Set menu item > **C-Sensor** < to > **yes** <

°C INT

Start

Stop

ⓘ In the start status the value „**C“** of the precision reference sensor is permanently shown in line 1.
The control indicator „°C“ in the header blinks.

In the stop status (OFF) it is in line 3.

ⓘ CONTROL –INTERNAL / EXTERNAL Control
The precision reference sensor cannot be used for external control.

Accesories:

Highly accurate temperature probe Order-No. 8 981 002

Technical specifications

Immersion depth		
minimum	90 mm	
maximum	140 mm	
Measurement range	-40,00 °C ... +300,00 °C	
Measurement accuracy		
Range	–40,00 °C .. . –0,001 °C	±(0,05 °C +0,05 % v. Mw.)
Range	0,00 °C .. +100,00 °C	±0,05 °C
Range	+100,001 °C .. +300,00 °C	±(0,05 °C +0,05 % v. Mw.)

9.5. Control

The circulator is designed for internal and external temperature control. This can be switched in this submenu. Only the set of parameters corresponding to the particular setting is displayed.

Control internal

```
2 CONTROL
 ------------------
→ControlType  intern
▼Selftuning   always
 Dynamic       aperio
 Xp              1.0K
 Tn              100s
 Tv               5s
 ------------------
```

Control external

```
2 CONTROL
 ------------------
→ControlType  extern
▼Selftuning   always
 CoSpeed        0.0
 Xp             0.7K
 Tn             720s
 Tv              55s
 Xpu            2.9K
 ------------------
```

MENU ↓

```
1 MAIN MENU
▲Configuration
→Control
▼Interface serial
```

OK ↓

ⓘ For external temperature control and measurement connect a Pt100 external sensor to the socket at the rear of the circulator.

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Parameter-Level	
2 CONTROL →ControlType intern ▼Selftuning always → OK ▼ ▲	2 CONTROL ControlType ⇕intern or 2 CONTROL ControlType ⇕extern	• Switch over control type by pressing ▲ ▼ and OK • Possible parameters: **intern / extern** ⓘ The control type can be adjusted in the **-OFF-** mode only.
2 CONTROL ▲ControlType intern →Selftuning always ▼Dynamic aperio → OK ▼ ▲	2 CONTROL Selftuning always	ⓘ The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters: **off** / **once** / **always**.

Control Type internal	Parameter-Level	
2 CONTROL ▲Selftuning always →Dynamic aperio ▼Xp 1.0K → OK ▼ ▲	2 CONTROL Dynamic aperio	ⓘ The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters: **aperio / normal** ⓘ This parameter affects the temperature sequence in case of internal control.

Control Type internal	Parameter-Level	
		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Example: 1 . 0 OK Setting range: 0.1 … 99.9 K
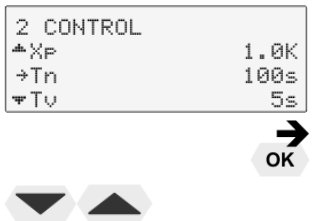		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 3 … 9999 s
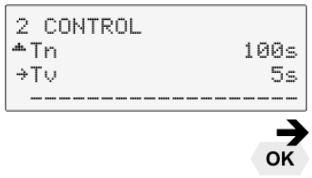		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 0 … 999 s
Control Type external	**Parameter-Level**	
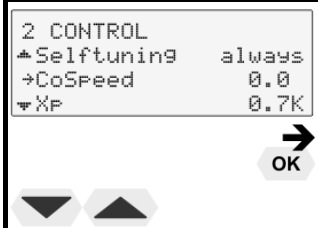		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Example: 0 . 0 OK Setting range: 0.0 … 5.0
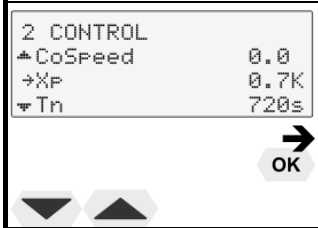		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 0.1 … 99.9 K
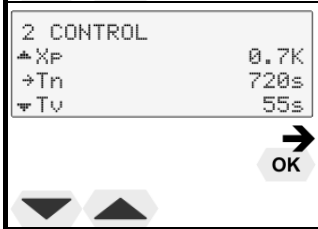		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 3 … 9999 s
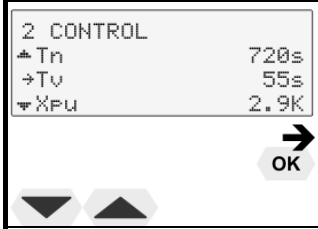		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 0 … 999 s
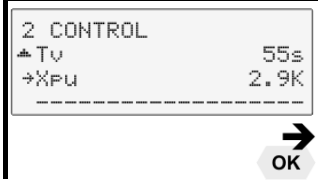		• The value flashes. Set by using the numeric keypad and confirm by pressing OK. Setting range: 0.1 … 99.9 K

9.5.1. Control internal / external

ⓘ The control type can be adjusted in the **-OFF-** mode only.

Possible parameters:

intern	internal temperature control
extern	external temperature control with external Pt100 sensor

ext.
Pt100

IMPORTANT:
Additional measures for external temperature control.

ⓘ Connect a Pt100 sensor to the socket on the rear of the circulator.

ⓘ Sensor calibration of the external Pt100 sensor is performed in the >ATCalibration< menu.

ⓘ Suggested adjustments for external temperature control:
Upper band / Lower band and IntMax / IntMin
see Section >Limits<.

ⓘ External temperature control does not allow the setpoint to be set via the “ext. Pt100” socket.

Notice:
Place the external sensor into the temperature-controlled medium and securely fix the sensor.

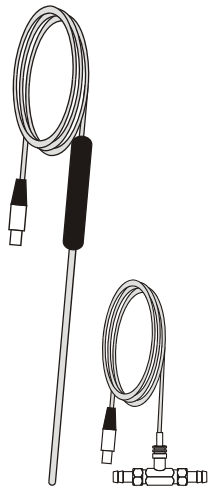

Pt100 M+R

Accessory: Pt100 external sensor

Order No.	Description	Material	Cable
8981003	200x6 mm Ø,	stainless steel	1.5 m
8981005	200x6 mm Ø,	glass	1.5 m
8981006	20x2 mm Ø,	stainless steel	1.5 m
8981010	300x6 mm Ø,	stainless steel	1.5 m
8981015	300x6 mm Ø,	stainless steel / PTFE coated	3 m
8981013	600x6 mm Ø,	stainless steel / PTFE coated	3 m
8981016	900x6 mm Ø,	stainless steel / PTFE coated	3 m
8981014	1200x6 mm Ø,	stainless steel / PTFE coated	3 m
8981103	Extension cable for Pt100 sensor		3.5 m
8981020	M+R in-line Pt100 sensor		

The M+R in-line Pt100 sensor is a flow sensor and can be installed loop circuit

9.5.2. Selftuning

When performing a selftuning for the controlled system (temperature application system), the control parameters Xp, Tn and Tv are automatically determined and stored.

Possible parameters:

off - no selftuning

The control parameters ascertained during the last identification are used for control purposes.

once - single selftuning (factory setting)

The instrument performs a single selftuning of the controlled system after each start with the OK key or after receiving a start command via the interface.

always - continual selftuning

The instrument performs a selftuning of the controlled system whenever a new setpoint is to be reached.

Use this setting only when the temperature application system changes permanently.

9.5.3. Dynamik intern

This parameter affects the temperature sequence only in case of internal control.

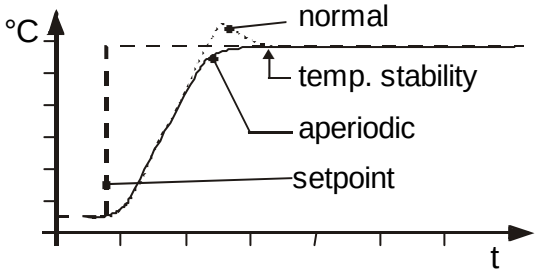

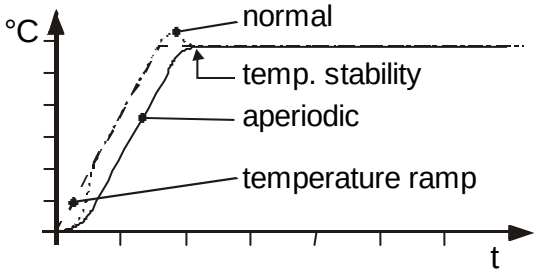

Factory setting: APER (aperiodic)

Possible parameters:

normal Allows for reaching the setpoint faster – with setpoint change or ramp function – but overshooting of up to 5 % is possible.

aperio Ramp function: the increase of temperature occurs temporally offset and achieves the target temperature without overshooting.
Setpoint change: The temperature increases at the same rate, the target temperature is achieved without overshooting.

ⓘ With both settings constant temperature is achieved after approximately the same time.

9.5.4. CoSpeed - extern

CoSpeed:

This parameter affects the temperature pattern only in case of **external** control.

Possible parameters: 0 ... 5

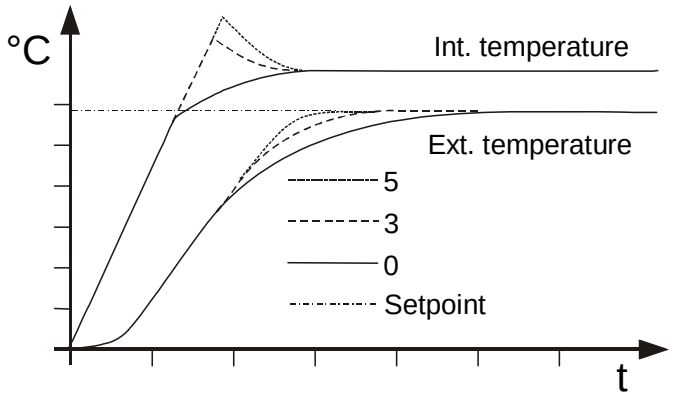

During selftuning, the control parameters Xp, Tn, and Tv of a controlled system are automatically determined and stored. The time required for tuning may vary depending on the controlled system. This controller design allows protection of sensitive objects requiring temperature control. As soon as a co-speed factor is set, it is considered in calculating the control parameters. As shown in the diagram, tuning times are shorter the higher the co-speed factor is, but overshoot can occur in the internal system.

9.5.5. Control parameters – internal/external

Control parameters – internal/external

The control parameters preset at the factory are in most cases adequate to achieve an optimal temperature pattern in the samples requiring temperature control.
Each parameter may be manually set via the keypad if necessary to allow optimal control performance.

Setting range:
internal / external
0.1 ... 99.9 K

Proportional range >Xp<

The proportional range is the temperature range below the setpoint temperature value in which the control circuit reduces the heating power from 100% to 0%.

Setting range:
internal / external
3 ...9999 s

Resetting time >Tn< (Integral component)

Compensation of the remaining control deviation due to proportional control. An insufficient resetting time may cause instabilities to occur. An excessive resetting time will unnecessarily prolong compensation of the control difference.

Setting range:
internal / external
0 ... 999 s

Lead time >Tv< (Differential component)

The differential component reduces the control settling time. An insufficient lead time will prolong the time required to compensate for disturbance effects and cause high overshoot during run-up. An excessive lead time could cause instabilities (oscillations) to occur.

Setting range:
0.1 ... 99.9 K

Proportional range >Xpu<

The proportional range Xpu of the cascaded controller is only needed for external control.

Optimization instructions for the PID control parameters:

optimum setting

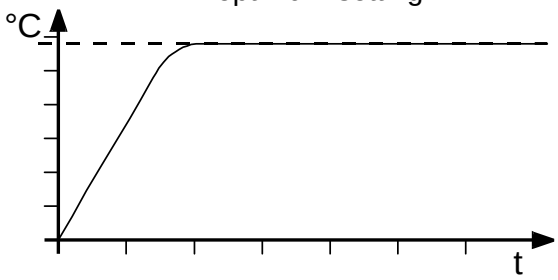

The heat-up curve reveals inappropriate control settings.

Inappropriate settings may produce the following heat-up curves:

Xp too low

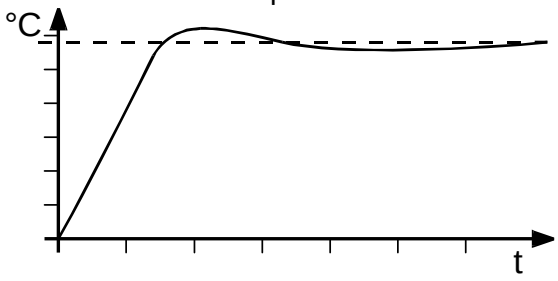

Tv/Tn too low

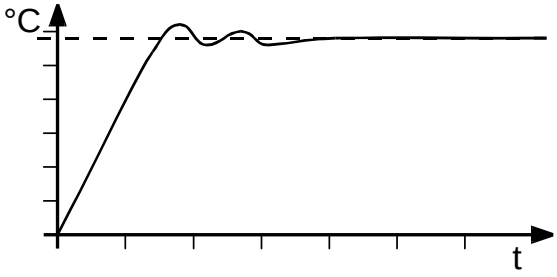

Xp too high or Tv too high

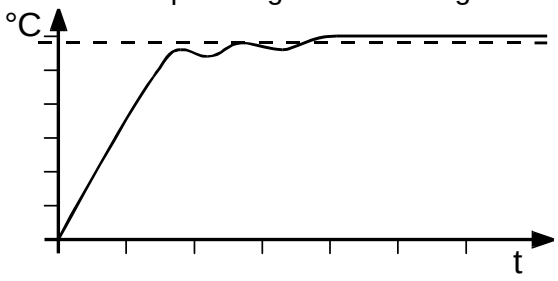

Tv/Tn too high or Xp too high

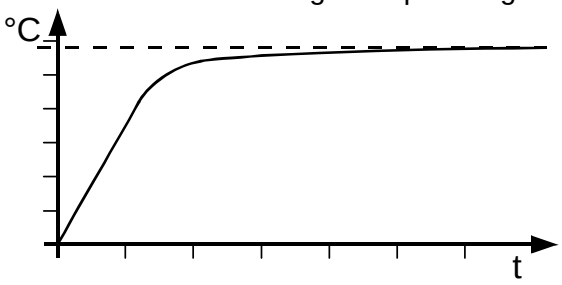

9.6. Serial Interface

Factory settings:
4800 Baud
even
hardware handshake

For communication between the circulator and a PC or a superordinated process system, the interface parameters of both units must be identical. The adjustment is usually carried out one time only in the >Interface serial< menu.

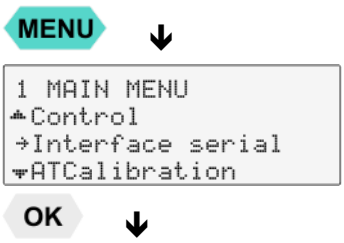

RS232

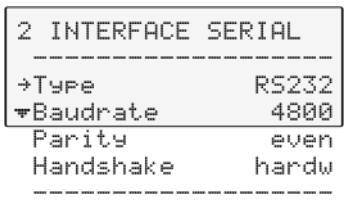

RS485

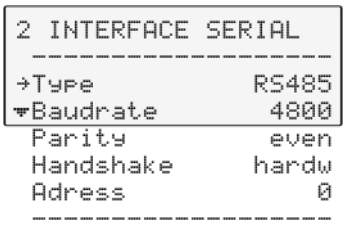

Level 2	Parameter-level	ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)
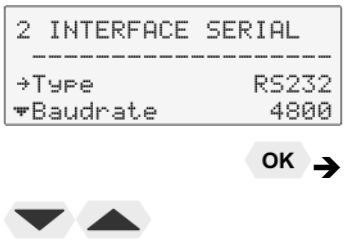		• The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters: **RS232 / RS485** **Address RS485:** 0 to 127
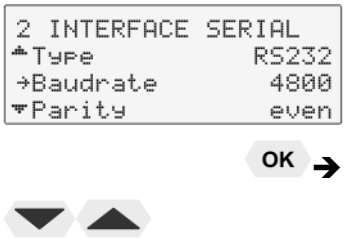		• The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters: **4800 / 9600 / 19200 / 38400**
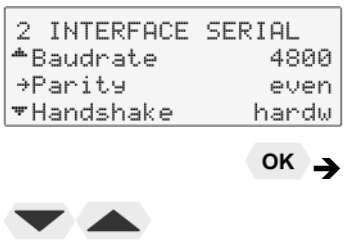		• The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters: **no/even/odd** even: Data bits = 7; Stop bits = 1 odd: Data bits = 7; Stop bits = 1 no: Data bits = 8; Stop bits = 1
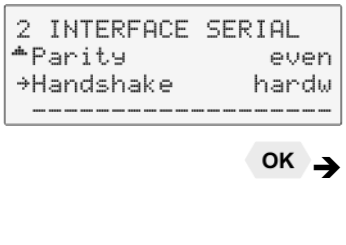		• The parameter flashes, switch by pressing ▲ ▼ and OK Possible parameters**: hardw / softw** Xon/Xoff-protocol (Software handshake) Protocol RTS/CTS (Hardware handshake)

9.7. ATC Absolute Temperature Calibration, 3-point calibration

ATC is used to compensate for a temperature difference between the circulator and a defined measuring point in the bath tank that may develop for physical reasons.

ATC internal

```
2 ATCalibration
 --------------------
→Sensor          intern
▼Status             no
  Type          3-point
  TmpValue1 : xx.xx°C
  CalValue1 : xx.xx°C
  TmpValue2 : xx.xx°C
  CalValue2 : xx.xx°C
  TmpValue3 : xx.xx°C
  CalValue3 : xx.xx°C
 --------------------
```

external

```
2 ATCalibration
 --------------------
→Sensor          extern
▼Status             no
  Type          3-point
  TmpValue1 : xx.xx°C
  CalValue1 : xx.xx°C
  TmpValue2 : xx.xx°C
  CalValue2 : xx.xx°C
  TmpValue3 : xx.xx°C
  CalValue3 : xx.xx°C
 --------------------
```

Example:
1-point calibration

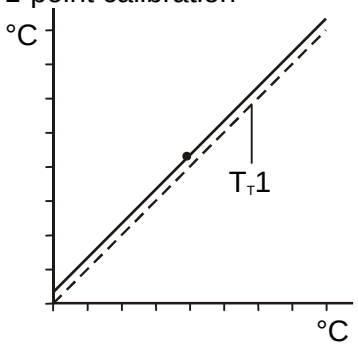

3-point calibration

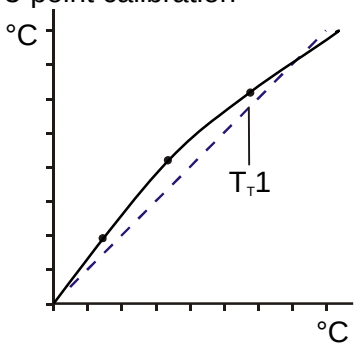

T_T 1 = Original curve

Principle:
For ATC calibration, in steady state the bath temperature at the location of the temperature sensor (CT) is determined at the respective adjusted working temperature. This value is then set on the circulator in the menu >ATCalibration< under menu item > CTEMP X <.
This can be a 1-point, 2-point or 3-point calibration.

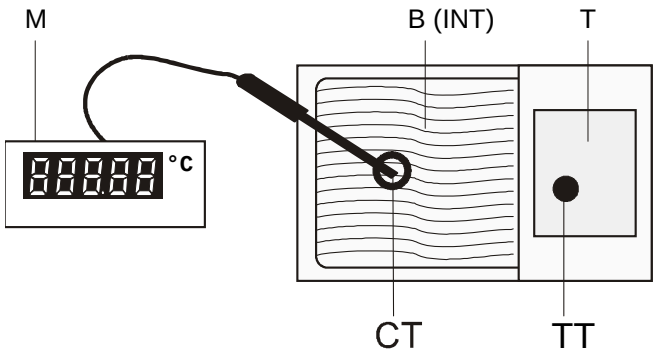

ATC (internal)

M = Temperature measuring instrument with temperature sensor
B = Bath tank (INTernal or EXTernal)
T = circulator

CT = Temperature on measuring point
TT = Temperature on circulator

MENU

```
1 MAIN MENU
↑Interface serial
→ATCalibration
↓Limits
```

OK

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Parameter-Level	
2 ATCalibration Sensor intern Status no OK → ▼ ▲	2 ATCalibration Sensor intern or 2 ATCalibration Sensor extern	• The parameter flashes, switch by pressing ▲ ▼ and OK
2 ATCalibration ↑Sensor intern →Status no ↓Type 3-point OK → ▼ ▲	2 ATCalibration Status yes or 2 ATCalibration Status no	ⓘ The parameter flashes, switch by pressing ▲ ▼ and OK ⓘ **>no<** Carry out an ATC calibration ⓘ **>yes<** return to standard operation after calibration.
2 ATCalibration ↑Status no →Type 3-point ↓TmpValue1 : xx.xx°C OK → ▼ ▲	2 ATCalibration Type 1-point 2 ATCalibration Type 2-point 2 ATCalibration Type 3-point	• The parameter flashes, switch by pressing ▲ ▼ and OK ⓘ A **>1-point<, >2-point<** or **>3-point< calibration** can be carried out.
2 ATCalibration ↑Type 3-Point →TmpValue1 : 80.00°C ↓CalValue1 : 79.70°C OK → ▼ ▲ 2 ATCalibration ↑TmpValue1 : xx.xx°C →CalValue1 : xx.xx°C ↓TmpValue2 : xx.xx°C OK → ▼ ▲	2 ATCalibration TmpValue1 : xx.xx°C ↩ 2 ATCalibration CalValue1 : xx.xx°C	The value >TmpValue< is only indicated ⓘ In addition the measured temperature value >CalValue X< is saved during the next step. • The value flashes. Set by using the numeric keypad and confirm by pressing OK.
	ⓘ If only a 1-point calibration is carried out, the following menu items are not indicated anymore	

2 ATCalibration CalValue1 : xx.xx°C TmpValue2 : xx.xx°C CalValue2 : xx.xx°C OK ➔	2 ATCalibration TmpValue2 : xx.xx°C	The value >TmpValue< is only indicated ⓘ In addition the measured temperature value >CalValue X< is saved during the next step.
2 ATCalibration TmpValue2 : xx.xx°C CalValue2 : xx.xx°C TmpValue3 : xx.xx°C OK ➔	2 ATCalibration CalValue2 : xx.xx°C	• The value flashes. Set by using the numeric keypad and confirm by pressing OK.
	ⓘ If only a 2-point calibration is carried out, the following menu items are not indicated anymore	
2 ATCalibration CalValue2 : xx.xx°C TmpValue3 : xx.xx°C CalValue3 : xx.xx°C OK ➔	2 ATCalibration TmpValue3 : xx.xx°C	The value >TmpValue< is only indicated. ⓘ In addition the measured temperature value >CalValue X< is saved during the next step.
2 ATCalibration TmpValue3 : xx.xx°C CalValue3 : xx.xx°C OK ➔	2 ATCalibration CalValue3 : xx.xx°C	• The value flashes. Set by using the numeric keypad and confirm by pressing OK.

9.7.1. ATC Fühler - intern / extern



In the first submenu the ATC function is set for the >intern< internal or the >extern< external temperature sensor.

Calibration can be carried out for the internal temperature sensor and for the external temperature sensor connected to the socket „ext. Pt100“. The circulator is able to save both parameter sets. However only the one which has been set under menu item > sensor < is displayed.

9.7.2. ATC Status - yes / no



In the second submenu the ATC function for the temperature sensor selected above is activated >yes< or deactivated >no<.

>yes< (factory setting) The controller of the circulator uses the original curve of the temperature sensor or the new curve measured during the ATC calibration.
Important: Set to **>NO<** during the calibration process

>no< An ATC calibration is to be carried out.
Important: Set to **>yes<** after calibration.

ⓘ In the > Status < >yes< the ATC calibration always affects the current working temperature; also the one set via interface.

9.7.3. Type 1 -/ 2 -/ 3 point

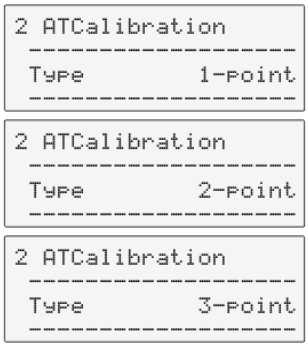

A **>1-point<, >2-point<** or **>3-point< calibration** can be carried out.

First geometrically define the location for calibration (measuring point CT), then determine the temperature values of the calibration points. The type of calibrations also determines the number of the following pairs of values indicated on the LCD DIALOG-DISPLAY.

Pairs of values:

TmpValue X: Circulator temperature 1 or 2 or 3 (actual value TT)
The actual temperature of the bath is simultaneously saved with the “calibration value“ >CalValue< and can be indicated for control purposes (value does not flash).

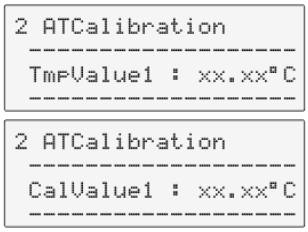

CalValue X: Calibration temperature 1 or 2 or 3 (actual value CT)
The „calibration value“ is determined with a temperature measuring device and saved under menu item >CalValue<.
(value flashes)

9.7.4. Example: 3-point calibration for internal control

In the temperature range from 80 °C to 160 °C the calibration curve of the temperature sensor (TT) is to be adjusted to the actual temperatures at measuring point (CT).

1. Set circulator to internal control:

ⓘ The type of control can be set only in the –OFF- mode.

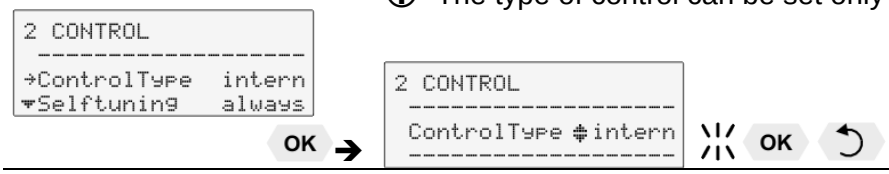

80.00 °C
120.00 °C
160.00 °C

2. Set working temperature setpoint

See standard display line 1

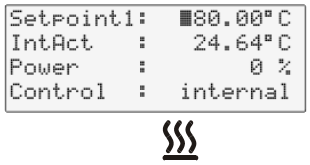

- Example 80.00 °C
  Press the keys 8 and 0 and confirm by pressing OK.
- The bath is heated up.
  Wait for approx. 5 minutes until the temperature is constant.

3. Reading of temperature measuring device



Read the value of measuring point CT on the device and enter under menu item > CalValue X< by using the keypad.

- CalValue 1< (79.70 °C)
- CalValue 2< (119.50 °C)
- CalValue 3< (159.30 °C)

4. Calibration

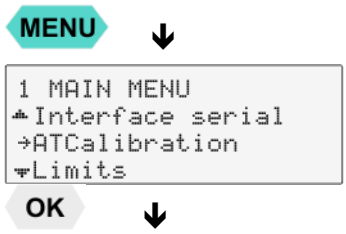

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

ⓘ 👁 Setting is required only for the first calibration point.

Level 2	Parameter-Level	
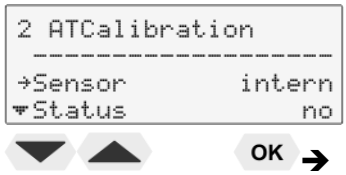	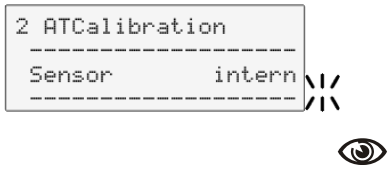	Set sensor: >intern<. • The parameter flashes, switch by pressing ▲ ▼ and OK
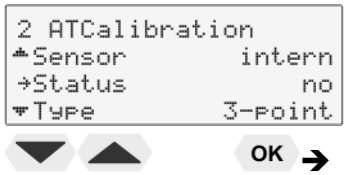	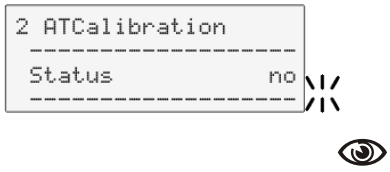	Set to >no< • The parameter flashes, switch by pressing ▲ ▼ and OK
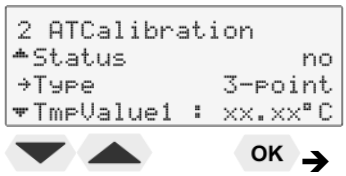	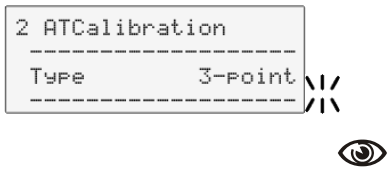	A >3-point< calibration is carried out. • The parameter flashes, switch by pressing ▲ ▼ and OK

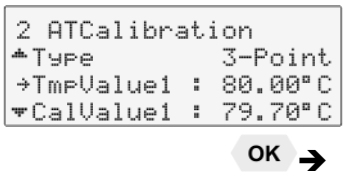 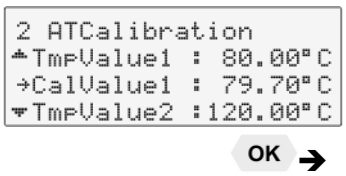 	 	The value >TmpValue< is only indicated. ⓘ In addition the measured temperature value >CalValue X< is saved during the next step. • The value flashes. Set by using the numeric keypad and confirm by pressing OK.
	Return to 2. Set working temperature value: 120.00 °C	
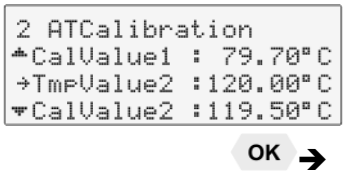 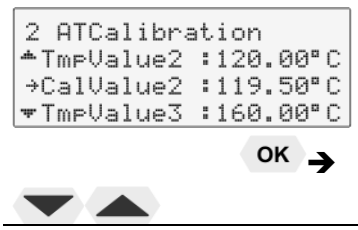 	 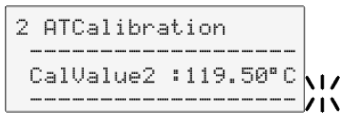	The value >TmpValue< is only indicated. ⓘ In addition the measured temperature value >CalValue X< is saved during the next step. • The value flashes. Set by using the numeric keypad and confirm by pressing OK.
	Return to 2. Set working temperature value: 160.00 °C	
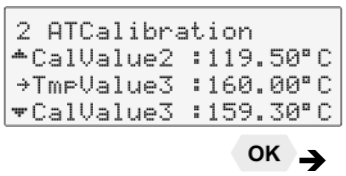 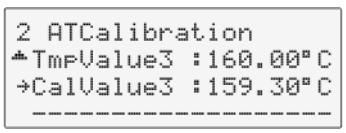	 	The value >TmpValue< is only indicated. ⓘ In addition the measured temperature value >CalValue X< is saved during the next step. • The value flashes. Set by using the numeric keypad and confirm by pressing OK.
	5. Return to standard operation	
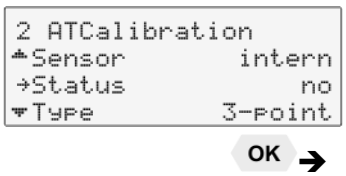		Set >YES< after calibration. (Standard operation) • The parameter flashes, switch by pressing ▲ ▼ and OK

9.8. Limits

The >Limits< menu allows the minimum and maximum values to be set for all important setting ranges and capacity variables.

Control internal

```
2 LIMITS
 ------------------
→SetMax      300.00°C
▼SetMin      -94.99°C
 HeatingMax      100%
 CoolingMax        0%
 ------------------
```

Control external

```
2 LIMITS
 ------------------
→SetMax      300.00°C
▼SetMin      -94.99°C
 HeatingMax      100%
 CoolingMax        0%
 IntMax       300.00°C
 IntMin       -94.99°C
 Upper band       200K
 Lower band       200K
 ------------------
```

MENU ↓

```
1 MAIN MENU
▲ATCalibration
→Limits
▼Inputs/Outputs
```

OK ↓

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK).

Level 2	Parameter-level	
2 LIMITS →SetMax 300.00°C ▼SetMin -94.99°C ▼ ▲ OK →	2 LIMITS SetMax 300.00°C	• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
2 LIMITS ▲SetMax 300.00°C →SetMin -94.99°C ▼HeatingMax 100% ▼ ▲ OK →	2 LIMITS SetMin -94.99°C	• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
2 LIMITS ▲SetMin -94.99°C →HeatingMax 100% ▼CoolingMax 0% ▼ ▲ OK →	2 LIMITS HeatingMax 100%	• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
2 LIMITS ▲HeatingMax 100% →CoolingMax 100% ▼IntMax 300.00°C ▼ ▲ OK →	2 LIMITS CoolingMax 0%	• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .

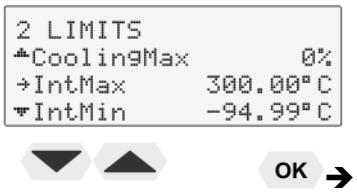		• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
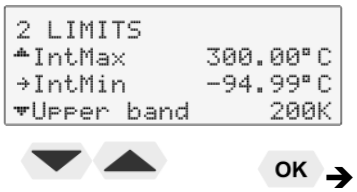		• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
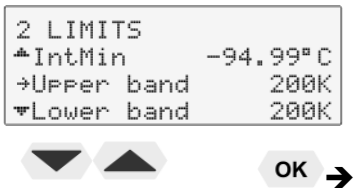		• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .
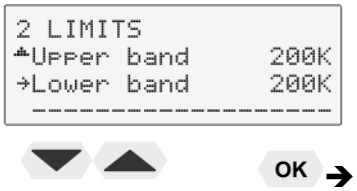		• The parameter flashes. Set by using the numeric keypad and confirm by pressing OK .

9.8.1. Limits for internal control and external control



Set Max / Min– Maximum and minimum setpoint
Restriction of the adjustable temperature range.

The limitation of the operating temperature range effects the temperature setting in the menu with the key T .

Only setting of working temperatures which lie within the determined limits is possible
Existing settings for Setpoint 1, -2, -3, as well as those for >OverTemp< and > SubTemp <, are automatically deferred into the limit range.

Setting range: -94,90 °C ... +300,0 °C

Set maximum heating / cooling

The heating and cooling capacity of the unit are adjustable. 100 % corresponds to the technical specification of the equipment.

Setting range:

Heating Max – 0 to 100 % in 1 % steps
Cooling Max – 0 to 100 % in 1 % steps

9.8.2. Limits for external control

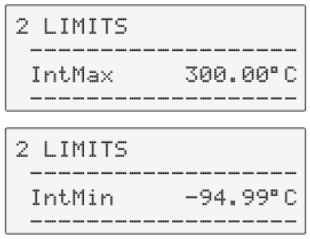



> **SAFETMP <**

INTERN MAX / MIN
Restriction for the temperature range of the internal bath.

Setting range: -94,9 °C ... +300,0 °C

The limits IntMax and IntMin are only active in external control. IntMax and IntMin determine fixed limits for the temperature within the internal bath. The temperature controller cannot exceed these limits even if it would be necessary for achieving the temperature in an external system. Therefore it is possible that the external setpoint cannot be achieved.

Sense of limit setting:

- ☑ Protects the bath fluid from overheating.
- ☑ Prevents an undesired alarm shutdown by the excess temperature protection - *>ALARM CODE 14<*.
  Set the value of > Int Max at least 5 °C below the value of **>SafeTemp<**.
- ☑ Protects the pump motor from high viscosity of the bath fluid at low temperatures.
- ☑ For refrigerated circulators. Freezing protection when using water as bath fluid.

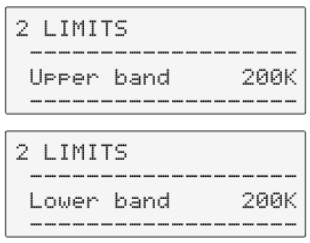

Upper band: and **Lower band**:

The band limitation is active during external control. Varied, practice-oriented setting are feasible for heat-up and cool-down phases.

Setting range: 0 °C ... 200 °C

Upper band: and **Lower band** allow for the limitation of the difference between the temperatures in the internal bath and the external system to any maximum value for the heat-up and cool-down phase.
During the heat-up phase this difference value is always added to the actual external temperature. During the cool-down phase the difference value is subtracted.

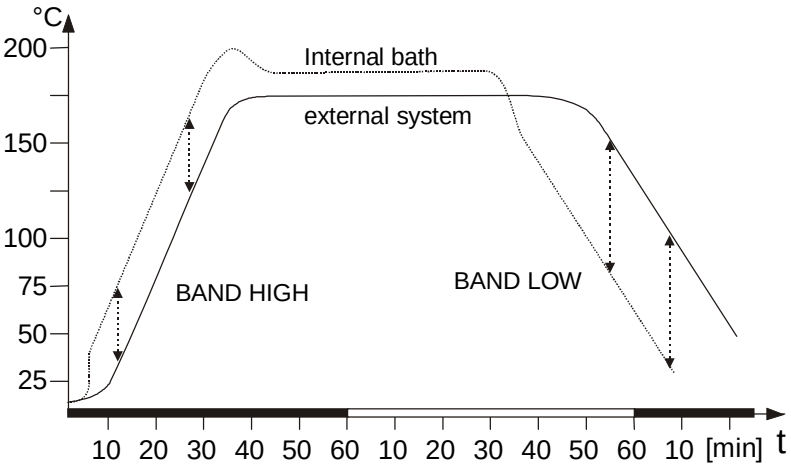

Sense of a band limitation:

- ☑ Protection of objects and samples by gentle temperature control
- ☑ Protection of e.g. glass reactors from thermal shock.

9.9. Analog inputs/outputs

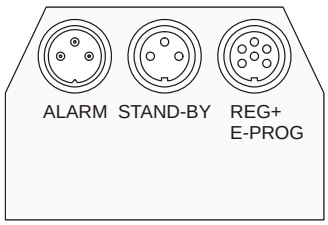

If the electronic module is not fitted, the item >inputs/outputs< will be missing in the menu.

ⓘ In order to use the analog inputs and outputs, the circulator must be equipped with the electronic module, which is available as option.
Order No. 8 900 100 Electronic module

This submenu enables the input and output values to be set for the programmer input and the temperature recorder outputs of the REG+E-PROG socket.

The >STAND-BY< input and the >ALARM< output are configurable.

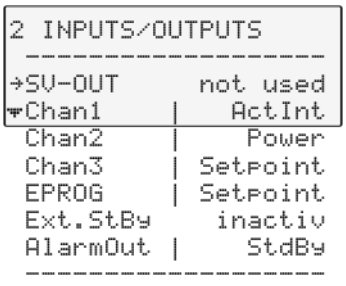

Menu item >SV-OUT< is not used.

Channel 1	voltage output for recorder	(V)
Channel 2	voltage output for recorder	(V))
Channel 3	current output for recorder	(mA)
EPROG	external programmer input	
External standby	Standby input (for external switch-off)	
Alarm output	Output for external alarm signal	

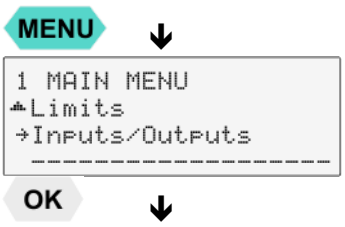

NOTE:
Channel 2 is pre-configured for the connection of an HST Booster Heater.

ⓘ Press the ↩ key if a parameter is to be retained. (prior to OK)

Level 2	Parameter-Level	
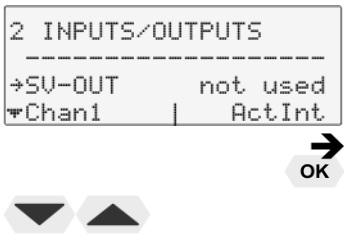		Menu item >SV-OUT< is not used.

Level 2	Level 3	Parameter-level
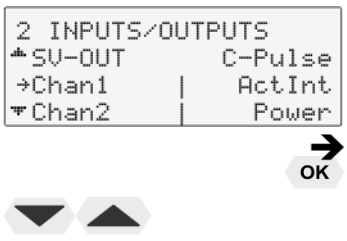	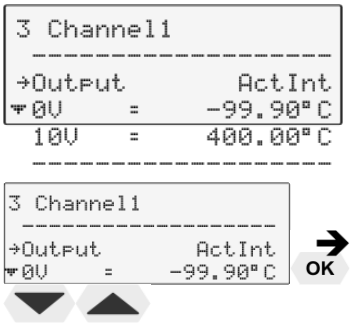	Define the output value for channel 1 Possible parameters: **ActInt, ActExt, Power, Setpoint** • The parameter flashes, switch by pressing ▲ ▼ and OK

Level 2	Level 3	Parameter-level
▼ ▲	3 Channel1 Output ActInt →0V = -99.90°C ▼10V = 400.00°C ▼ ▲ OK	Select the scale for channel 1. • The value flashes. Set by using the numeric keypad and confirm by pressing OK . 3 Channel1 0V = -99.90°C
	3 Channel1 0V = -99.90°C →10V = 400.00°C OK	• The value flashes. Set by using the numeric keypad and confirm by pressing OK . 3 Channel1 10V = 400.00°C
2 INPUTS/OUTPUTS Chan1 | ActInt →Chan2 | Power ▼Chan3 | Setpoint OK ▼ ▲	3 Channel2 →Output Power ▼0V = 0.00 % 10V = 100.00 % 3 Kanal2 →Output Power ▼0V = 0.00 % ▼ ▲ OK	Define the output value for channel 2. Possible parameters: **ActInt, ActExt, Power, Setpoint** • The parameter flashes, switch by pressing ▲ ▼ and OK 3 Channel2 Output ⇕ Power
	3 Channel2 Output Power →0V = 0.00 % ▼10V = 100.00 % ▼ ▲ OK	Select the scale for channel 2. • The value flashes. Set by using the numeric keypad and confirm by pressing OK . 3 Channel2 0V = 0.00 %
	3 Channel2 0V = 0.00 % →10V = 100.00 % OK	• The value flashes. Set by using the numeric keypad and confirm by pressing OK . 3 Channel2 10V = 100.00 %
2 INPUTS/OUTPUTS Chan2 | Power →Chan3 | Setpoint ▼EPROG | Setpoint OK ▼ ▲	3 Channel3 →Output Setpoint ▼0mA = -99.90°C 20mA = 400.00°C Region 0-20mA 3 Channel3 →Output Setpoint ▼0mA = -99.90°C ▼ ▲ OK	Define the output value for channel 3 Possible parameters: **ActInt, ActExt, Power, Setpoint** • The parameter flashes, switch by pressing ▲ ▼ and OK 3 Channel3 Output ⇕ Setpoint

Level 2	Level 3	Parameter-level
	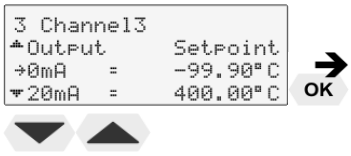	Select the scale for channel 3. • The value flashes. Set by using the numeric keypad and confirm by pressing **OK** . 
	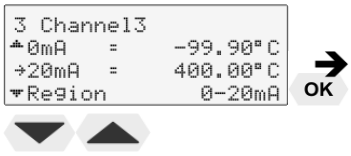	• The value flashes. Set by using the numeric keypad and confirm by pressing **OK** .
		Possible parameters: **0-20 mA, 4-20 mA** • The parameter flashes, switch by pressing and **OK**
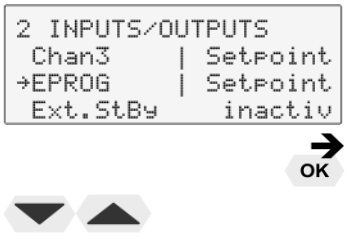	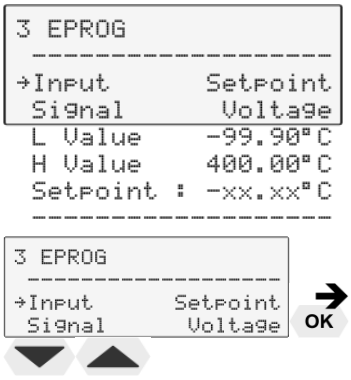	Possible parameters: **Setpoint, variable, flow rate, pressure** • The parameter flashes, switch by pressing and **OK** 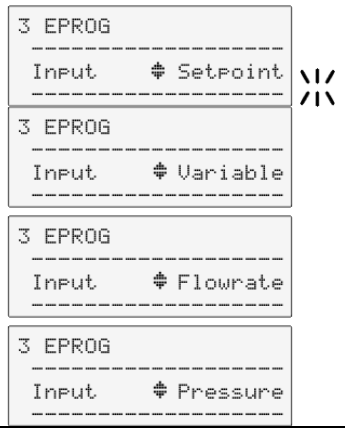
		Possible parameters: **voltage, current** • The parameter flashes, switch by pressing and **OK** 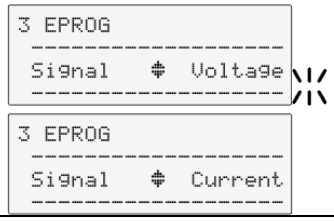

Level 2	Level 3	Parameter-level
	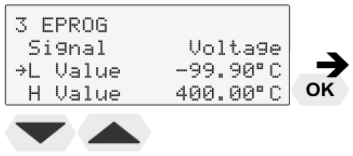	• The value flashes. Set by using the numeric keypad and confirm by pressing OK .
	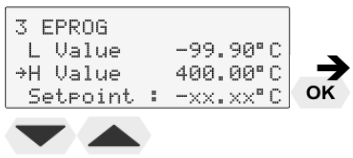	• The value flashes Set by using the numeric keypad and confirm by pressing OK . 
		ⓘ The value >setpoint< is only indicated. 
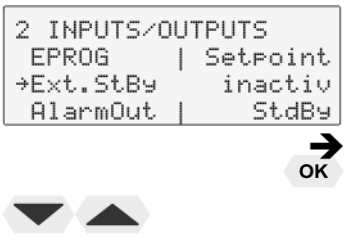	(Parameter Level) 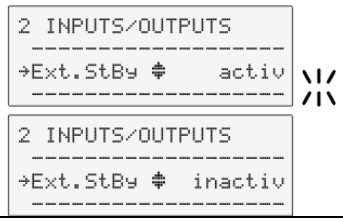	Possible parameters: **inactive, active** • The parameter flashes, switch by pressing and OK
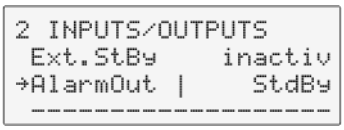	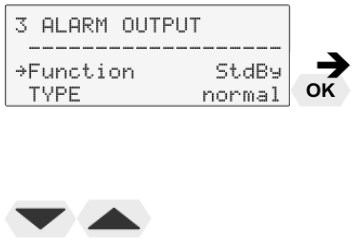	Possible parameters: **Alarm, Stand By, Alarm+ Stand By** • The parameter flashes, switch by pressing and OK 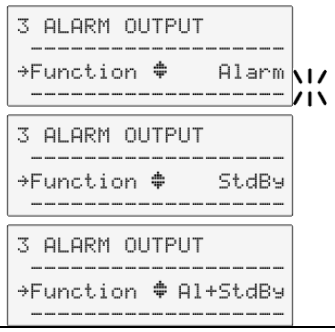
		Possible parameters: **normal, inverse** • The parameter flashes, switch by pressing and OK 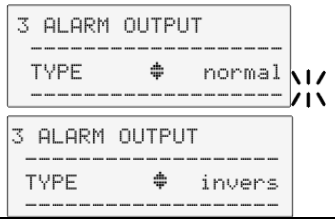

9.9.1. Outputs of the connector - REG+E-PROG

Outputs of the connector



1. <u>First define the desired output value for channels 1 to 3</u>:

   ActInt internal actual temperature value (bath temperature)
   ActExt external actual temperature value (external sensor)
   Power periodic or intermittent heating or cooling
   Setpoint active setpoint temperature
   (setpoint 1, 2, 3/integr. programmer/external programmer)

2. <u>Then select the scale for channels 1 to 3:</u>

   Voltage outputs channels 1 and 2
   Assign the voltage values of 0 V to the lowest and 10 V to the highest necessary temperature or power rating required as an output value (°C/%).
   Current output channel 3
   Assign the current values 0 mA or 4 mA to the lowest and 20 mA to the highest temperature or power rating required as an output value (°C/%).

3. The current output (channel 3) offers 2 ranges for selection:
   0 to 20 mA or 4 to 20 mA

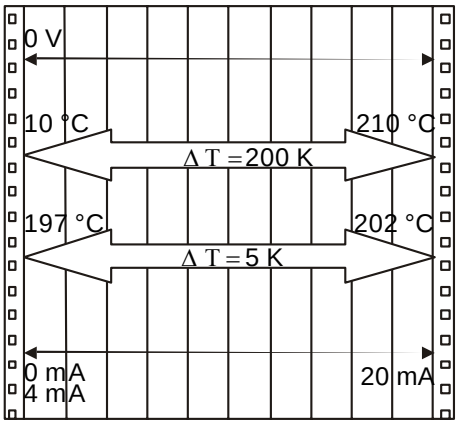

Examples:



lowest temperature value: 10 °C
highest temperature value 210 °C
Fig. shows 200 °C scaled to paper width
slope: 50 mV/°C

lowest temperature value: 197 °C
highest temperature value: 202 °C
Fig. shows 5 °C scaled to paper width
slope: 2000 mV/°C

9.9.2. Input of the connector - REG+E-PROG

Menu >Configuration<

1.
```
2 CONFIGURATION
▲Remote          off
→Setpoint ext  Eprog
▼Autostart       off
```

2.
```
2 CONFIGURATION
▲Off-Mode      P. off
→ActVar         Eprog
▼Time/Date
```

Menu >Inputs/Outputs<

3.
```
2 INPUTS/OUTPUTS
 Chan3     | Setpoint
→EPROG     | Flowrate
 Ext.StBy    inactiv
```

```
2 CONFIGURATION
 ------------------
→Remote          off
 Setpoint ext  Eprog
 Autostart       off
 Off-Mode     P. off
 ActVar         Eprog
 Time/Date
```

Example:

```
3 EPROG
 ------------------
→Input      Setpoint
 Signal      Current
 L Value      0.00°C
 H Value    300.00°C
 Setpoint :  50.00°C
 ------------------
```

E-PROG - Input

Setting is necessary if

1. the Setpoint is to be set via an external voltage or current source or programmer
   For this, in the menu >Configuration<, first set the menu item >Setpoint< to >Eprog<.
2. the heater variable should be controlled via an external control pulse.
   For this, in the menu >Configuration<, set the menu item > ActVar.< to >Eprog<.
3. the signal of an external flow meter should be registered.

ⓘ The E-Prog input can only be used either under menu item >**Setpoint**< or under menu item > **Actvar** <.
If the input is occupied neither by >**Setpoint**< or > **ActVar** <, the signal of a flow meter can be connected.

ⓘ First set menu >Configuration<, then menu >Inputs/Outputs<.

- Connect the external voltage or current source or programmer to the REG+E-PROG socket (12) of the circulator.

Selecting the signal:
The programmer (E-PROG) input of the circulator can be matched to the output signal of the external voltage or current source.

Voltage	voltage input
Current	current input

“L Value” - Setting the LOW value: (See below ➲)
First adjust and set the lowest voltage or current on the external voltage or current source (e.g., 0 V or 0 mA).
Then after approx. 30 seconds, enter the corresponding temperature value (e.g., 20.00°C).on the circulator by pressing the appropriate keys on the keypad and press **OK** to set.

“H Value” - **Setting the HIGH value:** (See below ➲)
First adjust and set the highest voltage or current on the external voltage or current source (e.g., 10 V or 20 mA).
Then after approx. 30 seconds, enter the corresponding temperature value (e.g., 300 °C).on the circulator by pressing the appropriate keys on the keypad and press **OK** to set.

Example:

ⓘ Set the external voltage or current source output for the equivalent of a 50 °C temperature setpoint.
The value adjusted and set on the external programmer is displayed in line 4 of the LCD DIALOG-DISPLAY for inspection.

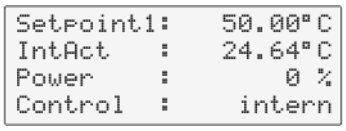

ⓘ After returning the LCD display to standard display by pressing the key ↩, the temperature value adjusted and set on the external voltage or current source is displayed in line 1
(Example: Eprog 50.00 °C).

This EPROG input enables the use of different voltage and current values as program parameters.

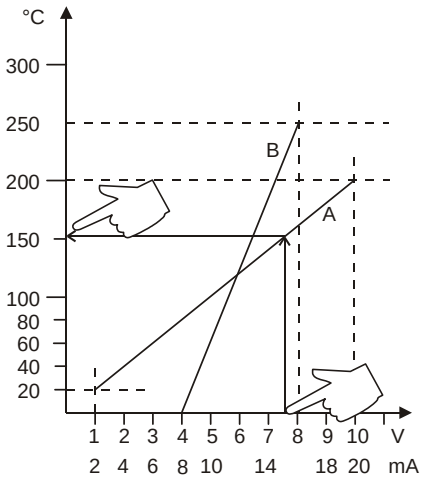

- **"L Value" - Setting the Low value:** (See below ➲)
  1) Adjust and set the lowest desired value on the voltage or current source (Example A: 1 V).
  Wait approximately 30 seconds.
  2) Assign a lower temperature threshold value to this adjusted voltage/current value by pressing the appropriate keys on the keypad of the instrument (Example A: 20 °C) and set by pressing OK .
- **"H Value" - Setting the High value:** (See below ➲)
  1) Adjust and set the highest desired value on the voltage or current source (Example A: 10 V).
  Wait approximately 30 seconds.
  2) Assign an upper temperature threshold value to this adjusted voltage/current value by pressing the appropriate keys on the keypad of the instrument
  (Example A: 200 °C) and set by pressing OK .

ⓘ Example B in the diagram illustrates that the end point values are freely selectable (e.g., 8 mA and 16 mA).

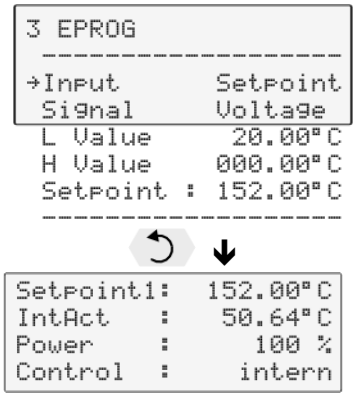

Example out of diagram A:

- Adjusting the voltage source for an output of 7.6 V!

Line 5 of the LCD DIALOG-DISPLAY shows the externally set setpoint value. The instrument calculates this value from the slope of the two specified end points (in example A, 7.6 V corresponds to an external setpoint temperature of 152.0 °C).

After returning the LCD display to standard display by pressing ↩, this value is displayed in line 1
(Example: EPROG 152.00 °C).

Notice:
If this adjustment is not correctly performed at two different points, the setpoint setting will be incorrect.

Important:
The usable temperature range between > **L Value** < and > **H Value** < is limited to the configured working temperature range of the circulator or unit combination. For the working temperature range, see technical specifications.

9.9.3. External Stand-by input

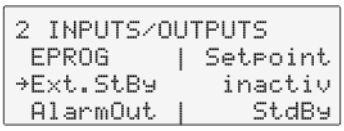

Ext. StBy (External STAND-BY input)

Stand-By input for external switch-off.

Possible parameters:

inactive - Stand-By input is ignored

active - Stand-By input is active

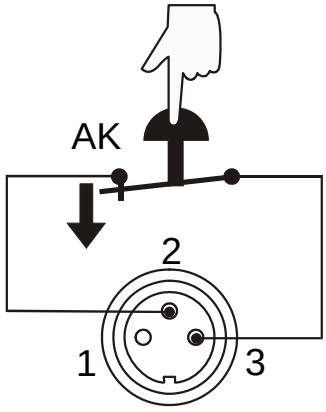

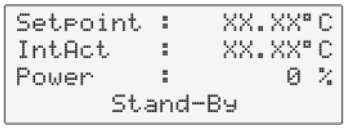

Activate the standby input:

1. Under menu item >**Ext. StBy**<, set the parameter to >**active<**.
2. Connect an external contact “AK” (e.g., for external switch-off) or an alarm contact of the superordinated system.

If the connection between pin 2 and pin 3 is interrupted by opening the contact “AK”, a complete shutdown of the circulating pump and heater is effected, and the unit enters the condition “**E OFF**”.
As long as the contact remains open, line 4 of the LCD DIALOG-DISPLAY flashes and displays the message “Stand-By”.

If the contact is reclosed, the instrument returns to the standby state and “ **E OFF** “ is displayed. Press OK to start.

ⓘ Additional tips for using the STAND-BY input:

The standby function can be used in conjunction with the AUTOSTART feature.

1. If the Autostart function is NOT turned ON, the standby input is used as described above.
2. If the Autostart function is enabled, the instrument will revert back to the original method of entering the setpoint (i.e., keypad, RS232, analog input, etc.).



Entering the setpoint with the keypad. e.g., T
As described above, a complete shutdown is accompanied by the “Stand-By” display and the OFF state. The programmable controller starts again when the contact is reclosed. The temperature of the bath fluid changed during the Stand-By state.

Entering the setpoint with the programmer.
The display “StandBy” appears. The setpoint value and the time are both held at the current value. The temperature of the bath fluid will be held constant at this temperature. The programmer continues once the contact is reclosed.

⚠ **Notice: this is not an actual emergency switch-off.**

9.9.4. Alarm-output



Alarm output (10)

(for external alarm signal)

This socket is a potential-free change-over contact. With the adjustments in the menu >Inputs/Outputs<, all operating conditions can be signaled without having to change the pin assignments.





Meaning of the terms under menu item >Function< :

The circulator is in condition

>StandBy<

or



>Alarm<



For >Type: normal<, pins 2 and 3 are connected in any case according to the selected >Function<.

For >Type: inverse<, pins 2 and 1 are connected in any case according to the selected >Function<.

Switching capacity	max.	30 W/40 VA
Switching voltage	max.	125 V~/–
Switching current	max.	1 A

10. Troubleshooting guide / Error messages

Alarm with complete shutdown:

If one of the following failures occur a complete, all-pole shutdown of the heater and circulating pump is effected.

„⚠“ lights up and a continuous signal sounds.
The code for the cause of alarm is indicated on the VFD COMFORT-DISPLAY.

Alarm without shutdown:

The code for the cause of alarm is indicated on the VFD COMFORT-DISPLAY. The warning signal sounds in regular intervals. The messages appear every 10 seconds.

- Press the key **OK** to stop the signal
- Press **OK** to indicate the help text in the LCD DIALOG-DISPLAY when alarm messages appear.



The circulator is operated without bath fluid, or the liquid level is insufficient. Replenish the bath tank with the bath fluid.

Tube breakage has occurred (insufficient filling level due to excessive bath fluid pumped out). Replace the tubing and replenish the bath tank with the bath fluid.

The float is defect (e. g., because damaged in transit). Repair by authorized JULABO service personnel.

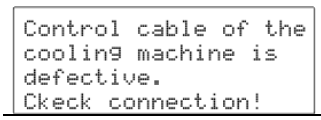

During the self-test after switch-on a short-circuit is registered between pin 2 and pin 4 of the control cable or the control cable is interrupted during operation.
Reconnect the cable or eliminate the short-circuit.

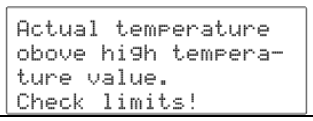

- Excess temperature warning
  or
  Excess temperature alarm

Warn-Type: Set to
>Warning< or >Alarm<

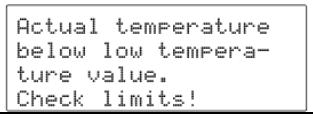

- Low temperature warning
  or
  Low temperature alarm.

Warn-Type: Set to
>Warning< or >Alarm<



The cable of the working temperature sensor is disconnected or short-circuited.

ALARM CODE 06 Sensor difference b. working- and safety-temp. Check pump stage and viscosity!	Defect of the working or excess temperature sensor. The working temperature and excess temperature sensors report a temperature difference of more than 35 K.
ALARM CODE 07 Internal hardware error. Call service!	Other errors (I^2C-BUS errors)
ALARM CODE 12 Error in A/D converter of the measuring system. Call service!	Error in A/D converter
ALARM CODE 14 Temperature exceeds the adjusted safety-temperature. Check adjustment!	Excess temperature sensor is defective. The safety temperature is below the working temperature setpoint. Set the safety temperature to a higher value.
ALARM CODE 15 External sensor is not connected or brocken. Check the external sensor!	External control selected, but external Pt100 sensor is not connected or is defective.
WARNING CODE 20	Cooling of the condenser is impaired. Clean the air-cooled condenser. For a water-cooled condenser, check the flow rate and temperature of the cooling water.
WARNING CODE 21	The first-stage compressor does not work. After a short cooling interval, the compressor motor will be automatically reconnected and the message “CODE 21” will no longer appear.
WARNING CODE 22	The second-stage compressor does not work. <u>Cooling compressor overload protection</u> The motor of the cooling compressor is equipped with an overload protector, which will be activated in case of excessive temperature in the capsule or excessive current draw. Causes of motor shut-off: - poor air circulation - short distance to walls - dirt accumulated on condenser - high ambient temperature - compressor switched off and on at short intervals
WARNING CODE 23	Excess temperature in the first-stage compressor.
WARNING CODE 24	Excess temperature in the second-stage compressor.

WARNING
CODE 25

Short-circuit in the control cable for the cooling machine during self-test.

ALARM
CODE 33

Internal safety-
temperature sensor
shorted/interrupted.
Call service!

Cable of the excess temperature sensor disconnected or short-circuited.

ALARM
CODE 38

Ext. sensor input
without signal but
setpoint programming
set to ext. Pt100!

Ext. Pt100 sensor input without signal, but setpoint programming set to external Pt100.

WARNING
CODE 40

The early warning system for low level signals a critical fluid level.
Replenish the bath tank with bath fluid.



After eliminating the malfunction, turn the mains power switch off and on again to cancel the alarm state.
If the unit cannot be returned to operation, contact an authorized JULABO service center.

CONFIGURATION
ERROR
CONFIRM BY
PRESSING : <OK>

Special message “CONFIGURATION ERROR”
The configuration of the circulator does not correspond to its present use.
Press **OK** to automatically perform a one-time modification of the configuration.
Then contact an authorized JULABO service center.

Disturbances that are not indicated.

The electronic pump motor is protected against overload by an electronic current limiter. If the viscosity of the bath fluid is or becomes too high, the motor stops running.



Fuses:

The mains fuses on the rear of the unit may easily be replaced as shown at left.
Circulator: Fine fuses (16a)– T 16 A, 250 V~ , D5 x 20 mm
Cooling machine: Fine fuses (16b)– T 10 A, 250 V~ , D5 x 20 mm

Warning:
Before exchanging the fuses, turn off the mains power switch and disconnect the power plug from the mains socket!
Only use fine fuses with a nominal value as specified.

Example:

Manufacturer	Supplier	Type	Order-No.
Schurter	Schurter	G-fuse link SPT T16A 5x20mm	No. 0001.2516

11. Electrical connections

Notice:

Use shielded cables only.
The shield of the connecting cable is electrically connected to the plug housing.

The unit ensures safe operation if connecting cables with a maximum length of 3 m are used. The use of longer cables does not affect proper performance of the unit, however external interferences may have a negative impact on safe operation (e.g. cellular phones).



Socket for external Pt100 sensor

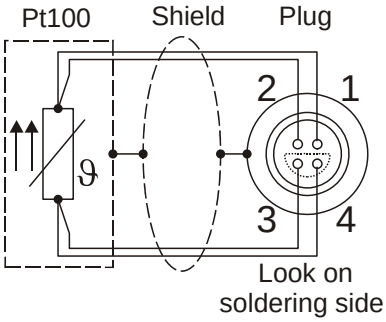

Pin assignment:

Pin	Signal
1	I+
2	U+
3	U-
4	I-

The shield of the connecting cable is electrically connected to the plug housing and the sensor tube.



RS232/RS485 serial interface

This port can be used to connect a computer with an RS232 or RS485 cable for remote control of the circulator.

Pin assignments RS232:

Pin 2	RxD	Receive Data
Pin 3	TxD	Transmit Data
Pin 5	0 V	Signal GND
Pin 7	RTS	Request to send
Pin 8	CTS	Clear to send

Pin 1; 4; 6, 9 Reserved - do not use!

Pin assignments RS485:

Pin 3	B	
Pin 5	0 V	Signal GND
Pin 6	+5 V (max. 50 mA)	
Pin 8	A	

Pin 1; 2; 4; 7; 9 Reserved - do not use!

Notice: RS485 serial interface

The max. load current between pin 5 and pin 6 is 50 mA.

RS232 interface cable

Circulator (9-pol)		PC (9-pol)
Pin 2 RxD	⇔	Pin 3 TxD
Pin 3 TxD	⇔	Pin 2 RxD
Pin 5 GND	⇔	Pin 5 GND
Pin 7 RTS	⇔	Pin 8 CTS
Pin 8 CTS	⇔	Pin 7 RTS

Accessories:	**Order No.**	**Description**
	8 980 073	RS232 interface cable 9-pol./9-pol. , 2,5 m
	8 900 110	USB interface adapter cable

❄ / Control output

The connector may only be used for control of a JULABO refrigerated circulator or JULABO MVS Solenoid valve controller for cooling water.



Pin assignment:

Pin	Signal (only with attached JULABO equipment)
1	+24 V (I max. current 25 mA)
2	0 V
3	Alarm relay
4	Reserved - do not use!
5	Cooling pulse

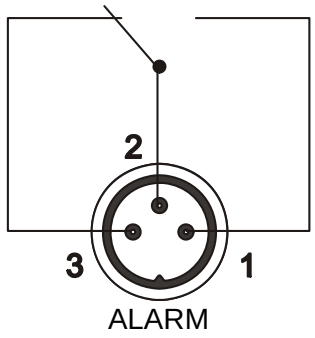

Alarm output

(for external alarm signal)

This potential-free change-over contact is activated in case of an alarm when pins 2 and 3 are connected.

Switching capacity	max.	30 W / 40 VA
Switching voltage	max.	125 V~/–
Switching current	max.	1 A

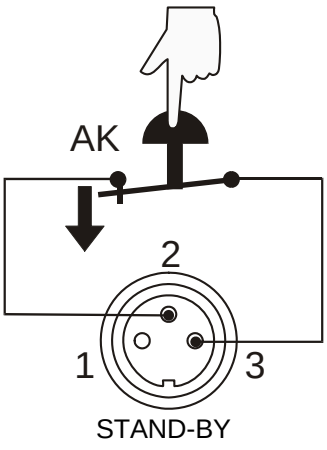

Stand-by input
(for external switch-off)

Pin assignment:

Pin	Signal
1	not connected
2	5 V / DC
3	0 V

REG+E-PROG

Programmer input / temperature recorder output

Pin			Signal
1	Voltage output	Channel 1	0 ... 10 V
2	Voltage output	Channel 2	0 ... 10 V
3	GND for outputs	0 V	
4	Programmer input	EPROG	0 to 10 V / 0 to 20 mA
5	Current output	Channel 3	0 to 20 mA / 4 to 20 mA
6	GND for Progammer	0 V	

12. Remote control

12.1. Setup for remote control



1. Check the interface parameters for both interfaces (on the circulator and PC) and make sure they match.
   In the >Interface< menu, set the menu item >Type< to >RS232< or >RS485<.
2. In the >Configuration< menu, set the menu item >Setpoint< to >RS232< or >RS485<.
3. Connect both units with an interface cable.

☞	Like all parameters that can be entered through the keypad, interface parameters are stored in the memory even after the circulator is turned off.

12.2. Communication with a PC or a superordinated data system

If the circulator is put into remote control mode via the configuration level, the VFD COMFORT-DISPLAY will read “R -OFF-” = REMOTE STOP. The circulator is now operated via the computer.
In general, the computer (master) sends commands to the circulator (slave). The circulator sends data (including error messages) only when the computer sends a query.

☞ In remote control mode, the start command and all values to be set must be resent by the PC via the interface in case of a power interruption. AUTOSTART is not possible.

A transfer sequence consists of:

- address (RS485 interface only)
- command
- space (⇔; Hex: 20)
- parameter (decimal separation with a period)
- end of file (↵; Hex: 0D)

- The response (data string) after an **in** command is always followed by a line feed (LF, Hex: 0A).

The commands are divided into **in** or **out** commands.
in commands: retrieve parameters
out commands: set parameters

Important times for a command transmission:

To ensure secure data transfer, the time gap between two commands should be at least 250 ms.
The circulator automatically responds to an **in** command with a data string followed by an LF (Line Feed). The next command should be sent only after 10 ms.

The **out** commands are valid only in remote control mode.

Examples:

When the RS485 interface is used, the three-digit instrument address precedes each command.
(example: address Ad32 = A**032**)

Command to set the working temperature >Setpoint1< to 55.5 °C

out_sp_00 ⇔ 55.5↵
A032_out_sp_00 ⇔ 55.5↵

Command to retrieve the working temperature >Setpoint1<

in_sp_00↵
A032_in_sp_00↵

Response from the circulator:

55.5↵ LF
A032_55.5↵ LF

Notice: out commands

Temperature values can be displayed on the circulator in °C or °F.
The settings sent via the interface must also be made in the selected unit according to this setting.

12.3. List of commands

out commands: Setting parameters or temperature values.

Command	Parameter	Response of circulator
out_mode_01	0	Use working temperature >Setpoint1<
out_mode_01	1	Use working temperature >Setpoint2<
out_mode_01	2	Use working temperature >Setpoint3<
out_mode_02	0	Selftuning “off”. Temperature control using the stored parameters.
out_mode_02	1	Selftuning “once” Single selftuning of the controlled system after the next start.
out_mode_02	2	Selftuning “always” Continual selftuning of the controlled system whenever a new setpoint is to be reached.

Command	Parameter	Response of circulator
out_mode_03	0	Set external programmer input to voltage. Voltage 0 V ... 10 V
out_mode_03	1	Set external programmer input to current. Current 0 mA ... 20 mA
out_mode_04	0	Temperature control of internal bath.
out_mode_04	1	External control with Pt100 sensor.
out_mode_05	0	Stop the unit = R –OFF-.
out_mode_05	1	Start the unit.
out_mode_08	0	Set the control dynamics - aperiodic
out_mode_08	1	Set the control dynamics - standard
out_sp_00	xxx.xx	Set working temperature. “Setpoint 1”
out_sp_01	xxx.xx	Set working temperature. “Setpoint 2”
out_sp_02	xxx.xx	Set working temperature. “Setpoint 3”
out_sp_03	xxx.xx	Set high temperature warning limit “OverTemp”
out_sp_04	xxx.xx	Set low temperature warning limit “SubTemp”
out_sp_06	xxx.xx	Set manipulated variable for heater via serial interface -100 ... +100 [%]
out_sp_07	x	Set the pump pressure stage. (1 ... 4)
out_par_04	x.x	CoSpeed for external control 0 ... 5.0.
out_par_06	xxx	Xp control parameter of the internal controller. 0.1 ... 99.9
out_par_07	xxx	Tn control parameter of the internal controller. 3 ... 9999
out_par_08	xxx	Tv control parameter of the internal controller. 0 ... 999
out_par_09	xxx	Xp control parameter of the cascade controller. 0.1 ... 99.9
out_par_10	xxx	Proportional share of the cascade controller. 1 ... 99.9
out_par_11	xxx	Tn control parameter of the cascade controller. 3 ... 9999
out_par_12	xxx	Tv control parameter of the cascade controller. 0 ... 999
out_par_13	xxx	Maximum internal temperature of the cascade controller.
out_par_14	xxx	Minimum internal temperature of the cascade controller.
out_par_15	xxx	Band limit (upper) 0 ... 200 °C
out_par_16	xxx	Band limit (lower) 0 ... 200 °C
out_hil_00	-xxx	Set the desired maximum cooling power (0% to 100%). **Note:** Enter the value with a preceding negative sign! This setting is meaningful only for FP cooling machines.
out_hil_01	xxx	Set the desired maximum heating power (10% to 100%).

in commands: Asking for parameters or temperature values to be displayed.

Command	Parameter	Response of circulator
version	None	Version number of the software (V X.xx)
status	none	Status message, error message (see page 85)
in_pv_00	none	Current bath temperature.
in_pv_01	none	Heating power being used (%).
in_pv_02	none	Temperature value registered by the external Pt100 sensor.
in_pv_03	none	Temperature value registered by the safety sensor.
in_pv_04	none	Setpoint temperature (“SafeTemp”) of the excess temperature protection
in_sp_00	none	Working temperature “Setpoint 1”
in_sp_01	none	Working temperature “Setpoint 2”
in_sp_02	none	Working temperature “Setpoint 3”
in_sp_03	none	High temperature warning limit “OverTemp”
in_sp_04	none	Low temperature warning limit “SubTemp”
in_sp_05	none	Setpoint temperature of the external programmer (REG+E-PROG).
in_sp_06	none	Temperature indication in °C or °F
in_sp_07	none	1. Adjusted pump stage in the -OFF- condition. 2. Pump stage corresponding to the effective rotational speed after start.
in_sp_08	none	Value of a flow rate sensor connected to the E-Prog input
in_sp_09	none	Value of a pressure sensor connected to the E-Prog input
in_par_00	none	Temperature difference between working sensor and safety sensor
in_par_01	none	Te - Time constant of the external bath.
in_par_02	none	Si - Internal slope
in_par_03	none	Ti - Time constant of the internal bath.
in_par_04	none	CoSpeed - Band limit (max. difference between the temperatures in the internal bath and external system).
in_par_05	none	Factor pk/ph0: Ratio of max. cooling capacity to max. heating capacity
in_par_06	none	Xp control parameter of the internal controller.
in_par_07	none	Tn control parameter of the internal controller.

Command	Parameter	Response of circulator
in_par_08	none	Tv control parameter of the internal controller.
in_par_09	none	Xp control parameter of the cascade controller.
in_par_10	none	Proportional share of the cascade controller.
in_par_11	none	Tn control parameter of the cascade controller.
in_par_12	none	Tv control parameter of the cascade controller.
in_par_13	none	Adjusted maximum internal temperature of the cascade controller.
in_par_14	none	Adjusted minimum internal temperature of the cascade controller.
in_par_15	none	Band limit (upper)
in_par_16	none	Band limit (lower)
in_mode_01	none	Selected setpoint: 0 = Setpoint 1 1 = Setpoint 2 2 = Setpoint 3
in_mode_02	none	Selftuning type: 0 = Selftuning “off” 1 = Selftuning “once” 2 = Selftuning “always”
in_mode_03	none	Type of external programmer input: 0 = Voltage 0 V to 10 V 1 = Current 0 mA to 20 mA
in_mode_04	none	Internal/external temperature control: 0 = Temperature control with internal sensor. 1 = Temperature control with external Pt100 sensor.
in_mode_05	none	Circulator in stop/start condition: 0 = stop 1 = start
in_mode_08	none	Adjusted control dynamics 0 = aperiodic 1 = standard
in_hil_00	none	Max. cooling power (%).
in_hil_01	none	Max. heating power (%).

12.4. Status messages

Status messages	Description
00 MANUAL STOP	Circulator in „OFF“ state.
01 MANUAL START	Circulator in keypad control mode.
02 REMOTE STOP	Circulator in „r OFF“ state.
03 REMOTE START	Circulator in remote control mode.

12.5. Error messages

Error messages	Description
-01 LOW LEVEL ALARM	Low liquid level alarm
-02 REFRIGERATOR ALARM	Control cable of the refrigerated circulator or MVS solenoid valve controller short-circuited or disconnected.
-03 EXCESS TEMPERATURE WARNING	High temperature warning
-04 LOW TEMPERATURE WARNING	Low temperature warning.
-05 WORKING SENSOR ALARM	Working temperature sensor short-circuited or disconnected.
-06 SENSOR DIFFERENCE ALARM	Sensor difference alarm. Working temperature and safety sensors report a temperature difference of more than 35 K.
-07 I^2C-BUS ERROR	Internal error when reading or writing the I^2C bus.
-08 INVALID COMMAND	Invalid command.
-09 COMMAND NOT ALLOWED IN CURRENT OPERATING MODE	Invalid command in current operating mode.
-10 VALUE TOO SMALL	Entered value too small.
-11 VALUE TOO LARGE	Entered value too large.
-12 TEMPERATURE MEASUREMENT ALARM	Error in A/D converter.
-13 WARNING : VALUE EXCEEDS TEMPERATURE LIMITS	Value lies outside the adjusted range for the high and low temperature warning limits. But the value is stored.
-14 EXCESS TEMPERATURE PROTECTOR ALARM	Excess temperature protector alarm
-15 EXTERNAL SENSOR ALARM	External control selected, but external Pt100 sensor not connected.

Error messages	Description
-20 WARNING: CLEAN CONDENSOR OR CHECK COOLING WATER CIRCUIT OF REFRIGERATOR	Cooling of the condenser is impaired. Clean air-cooled condenser. Check the flow rate and cooling water temperature for a water-cooled condenser.
-21 WARNING: COMPRESSOR STAGE 1 DOES NOT WORK	First-stage compressor does not work.
-22 WARNING: COMPRESSOR STAGE 2 DOES NOT WORK	Second-stage compressor does not work.
-23 WARNING: HIGH TEMPERATURE ON COMPRESSOR STAGE 1	Excess temperature at first-stage compressor.
-24 WARNING: HIGH TEMPERATURE ON COMPRESSOR STAGE 2	Excess temperature at second-stage compressor.
-25 REFRIGERATOR WARNING	Error in the cooling machine.
-26 WARNING: STAND-BY PLUG IS MISSING	External standby contact is open.
-30 CONFIGURATION ERROR: CONFIRM BY PRESSING <OK> ON CIRCULATOR	The configuration of the circulator does not correspond to its present use. Press OK to automatically perform a one-time modification of the configuration.
-33 SAFETY SENSOR ALARM	Excess temperature sensor short-circuited or disconnected.
-38 EXTERNAL SENSOR SETPOINT PROGRAMMING ALARM	Ext. Pt100 sensor input without signal and setpoint programming set to external Pt100.
-40 NIVEAU LEVEL WARNUNG	Low liquid level warning in the internal reservoir.

13. Installation of electronic module with analog connectors

Caution:
Always turn off the unit and disconnect the mains cable from the power source before performing any service or maintenance procedures, or before moving the unit. Configuration, installation, maintenance, and repairs on the circulator may be performed only by qualified personnel.

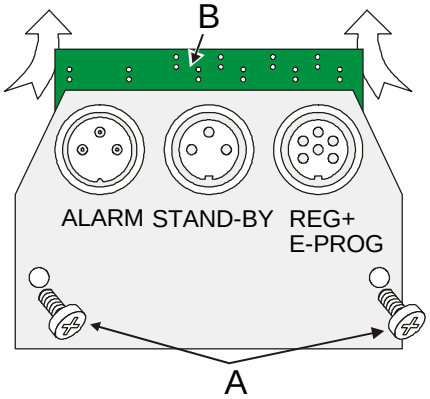

- Turn off the unit with the mains switch and disconnect the power plug.
- Remove the screws (A) and remove the dummy plate.
- Carefully insert the upper edge (B) into the rear panel from below, align the electronic module at the top and bottom, and connect the 15-pin connector by applying light pressure.
- Attach the electronic module using the screws (A).
- The circulator is ready for use. It automatically recognizes the installed electronic module.

14. JULABO Service – Online remote diagnosis

JULABO circulators of the HighTech series are equipped with a black box. This box is implemented in the controller and records all significant data for the last 30 minutes.
In case of a failure, this data can be read out from the unit by using special software. This software is available as a **free** download from www.julabo.de \ EasyBlackBox.

- Installation is easy and is performed step by step.
  Please observe the instructions.

- Data read-out is possible in the conditions “OFF”, “R OFF” or “ALARM”.
- Connect the circulator to the computer using an interface cable.
- Start the EasyBlackBox program.
  The program asks for the port used (COM1, ...) and the baud rate of the unit.
  You do not have this information on hand?
  Simply try it out!
  The program continues to send the request until the correct settings are made.

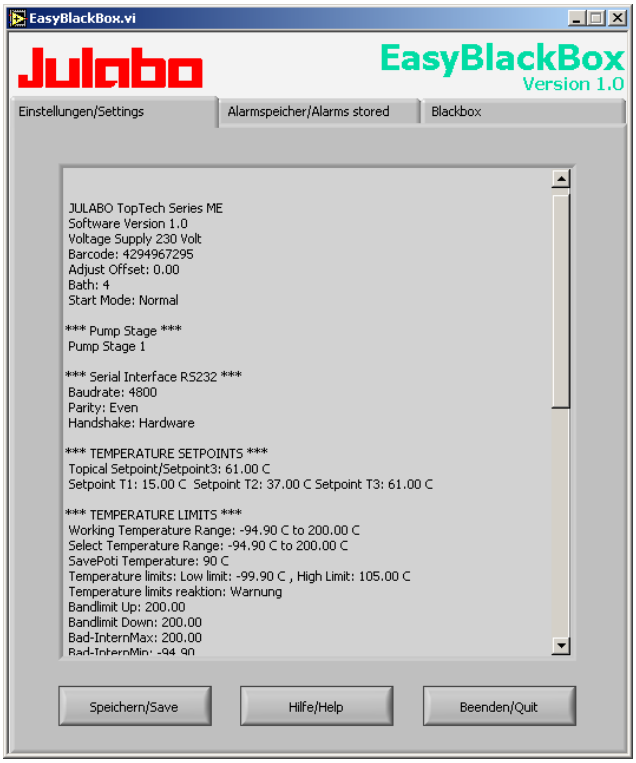

- Data is read out and shown on the monitor divided into the sections
  >Einstellungen/Settings<,
  >Alarmspeicher/Alarms stored<,
  >Blackbox<

  ← see example

- After pressing >Speichern/Save<, a text file is created. The program suggests a filename - >C:\model description and barcode no.<. Modifications are possible.
- E-mail this file to service@julabo.de, JULABO's service department. JULABO is thus able to provide rapid support.

15. Cleaning / repairing the unit

Caution:

- Always turn off the unit and disconnect the mains cable from the power source before cleaning the unit.
- Prevent humidity from entering into the circulator.
- Electrical connections and any other work must be performed by qualified personnel only.

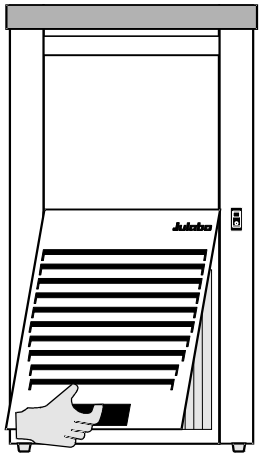

In dusty environments, the refrigerating machine's condenser should be cleaned by vacuuming every 1 to 2 months. The condenser is located behind the venting grid on the front of the unit.

- Switch off the unit, disconnect mains power cable.
- Remove the venting grid.
- Clean the ribbed condenser with a vacuum cleaner.
- Replace the venting grid.
- Switch on the unit.

Cleaning:

For cleaning the bath tank and the immersed parts of the circulator, use low surface tension water (e.g., soap suds).
Clean the outside of the unit using a wet cloth and low surface tension water.

The circulator is designed for continuous operation under normal conditions. Periodic maintenance is not required.

The tank should be filled only with a bath fluid recommended by JULABO. To avoid contamination, it is essential to change the bath fluid from time to time.

Repairs

Before asking for a service technician or returning a JULABO instrument for repair, please contact an authorized JULABO service station.

When returning the unit:

- Clean the unit in order to avoid any harm to the service personnel.
- Attach a short fault description.
- During transport the unit has to stand upright. Mark the packing correspondingly.
- When returning a unit, take care of careful and adequate packing.
- JULABO is not responsible for damages that might occur from insufficient packing.

JULABO reserves the right to carry out technical modifications with repairs for providing improved performance of a unit.